


Sample information

Sample Name:	Probka_3	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP_150317
Vial:	3	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-03-15 14:21:37 CET		
Processed:	2017-03-25 12:32:32 CET		

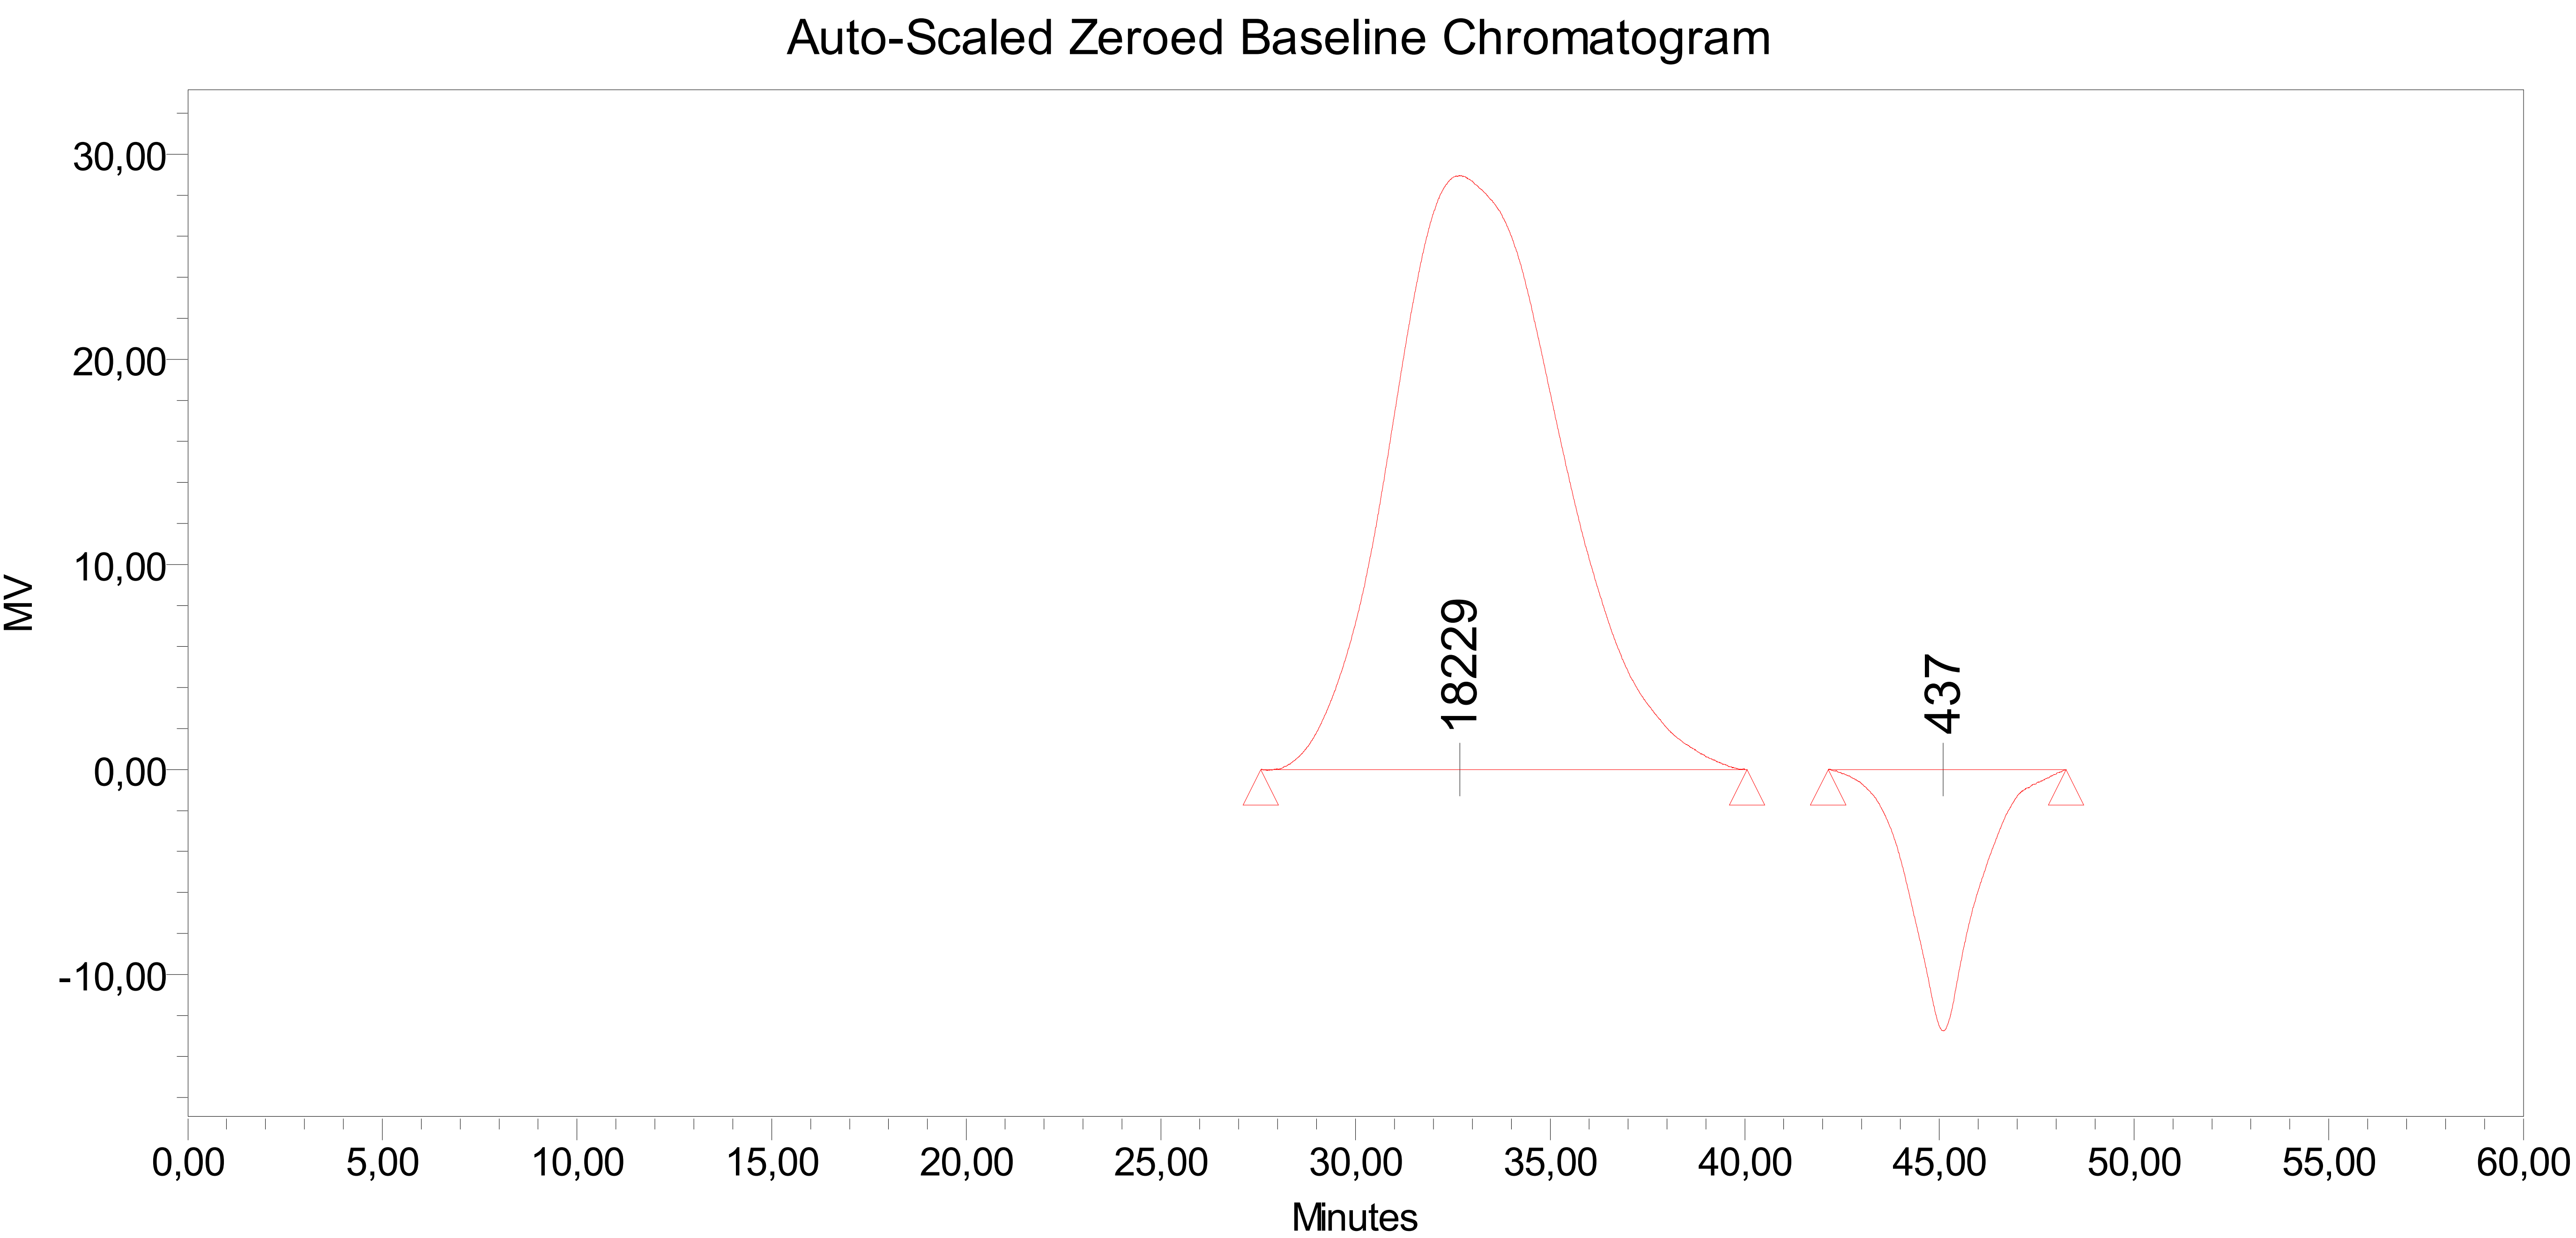

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	32,681	13474	21340	18229	35510	1,584	85,46
2	45,102	415	447	437	479	1,075	14,54

GPC Calibration Plot

