


Sample information

Sample Name:	Probka_31	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP021017
Vial:	4	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-10-02 13:32:15 CEST		
Processed:	2017-10-03 09:26:01 CEST		

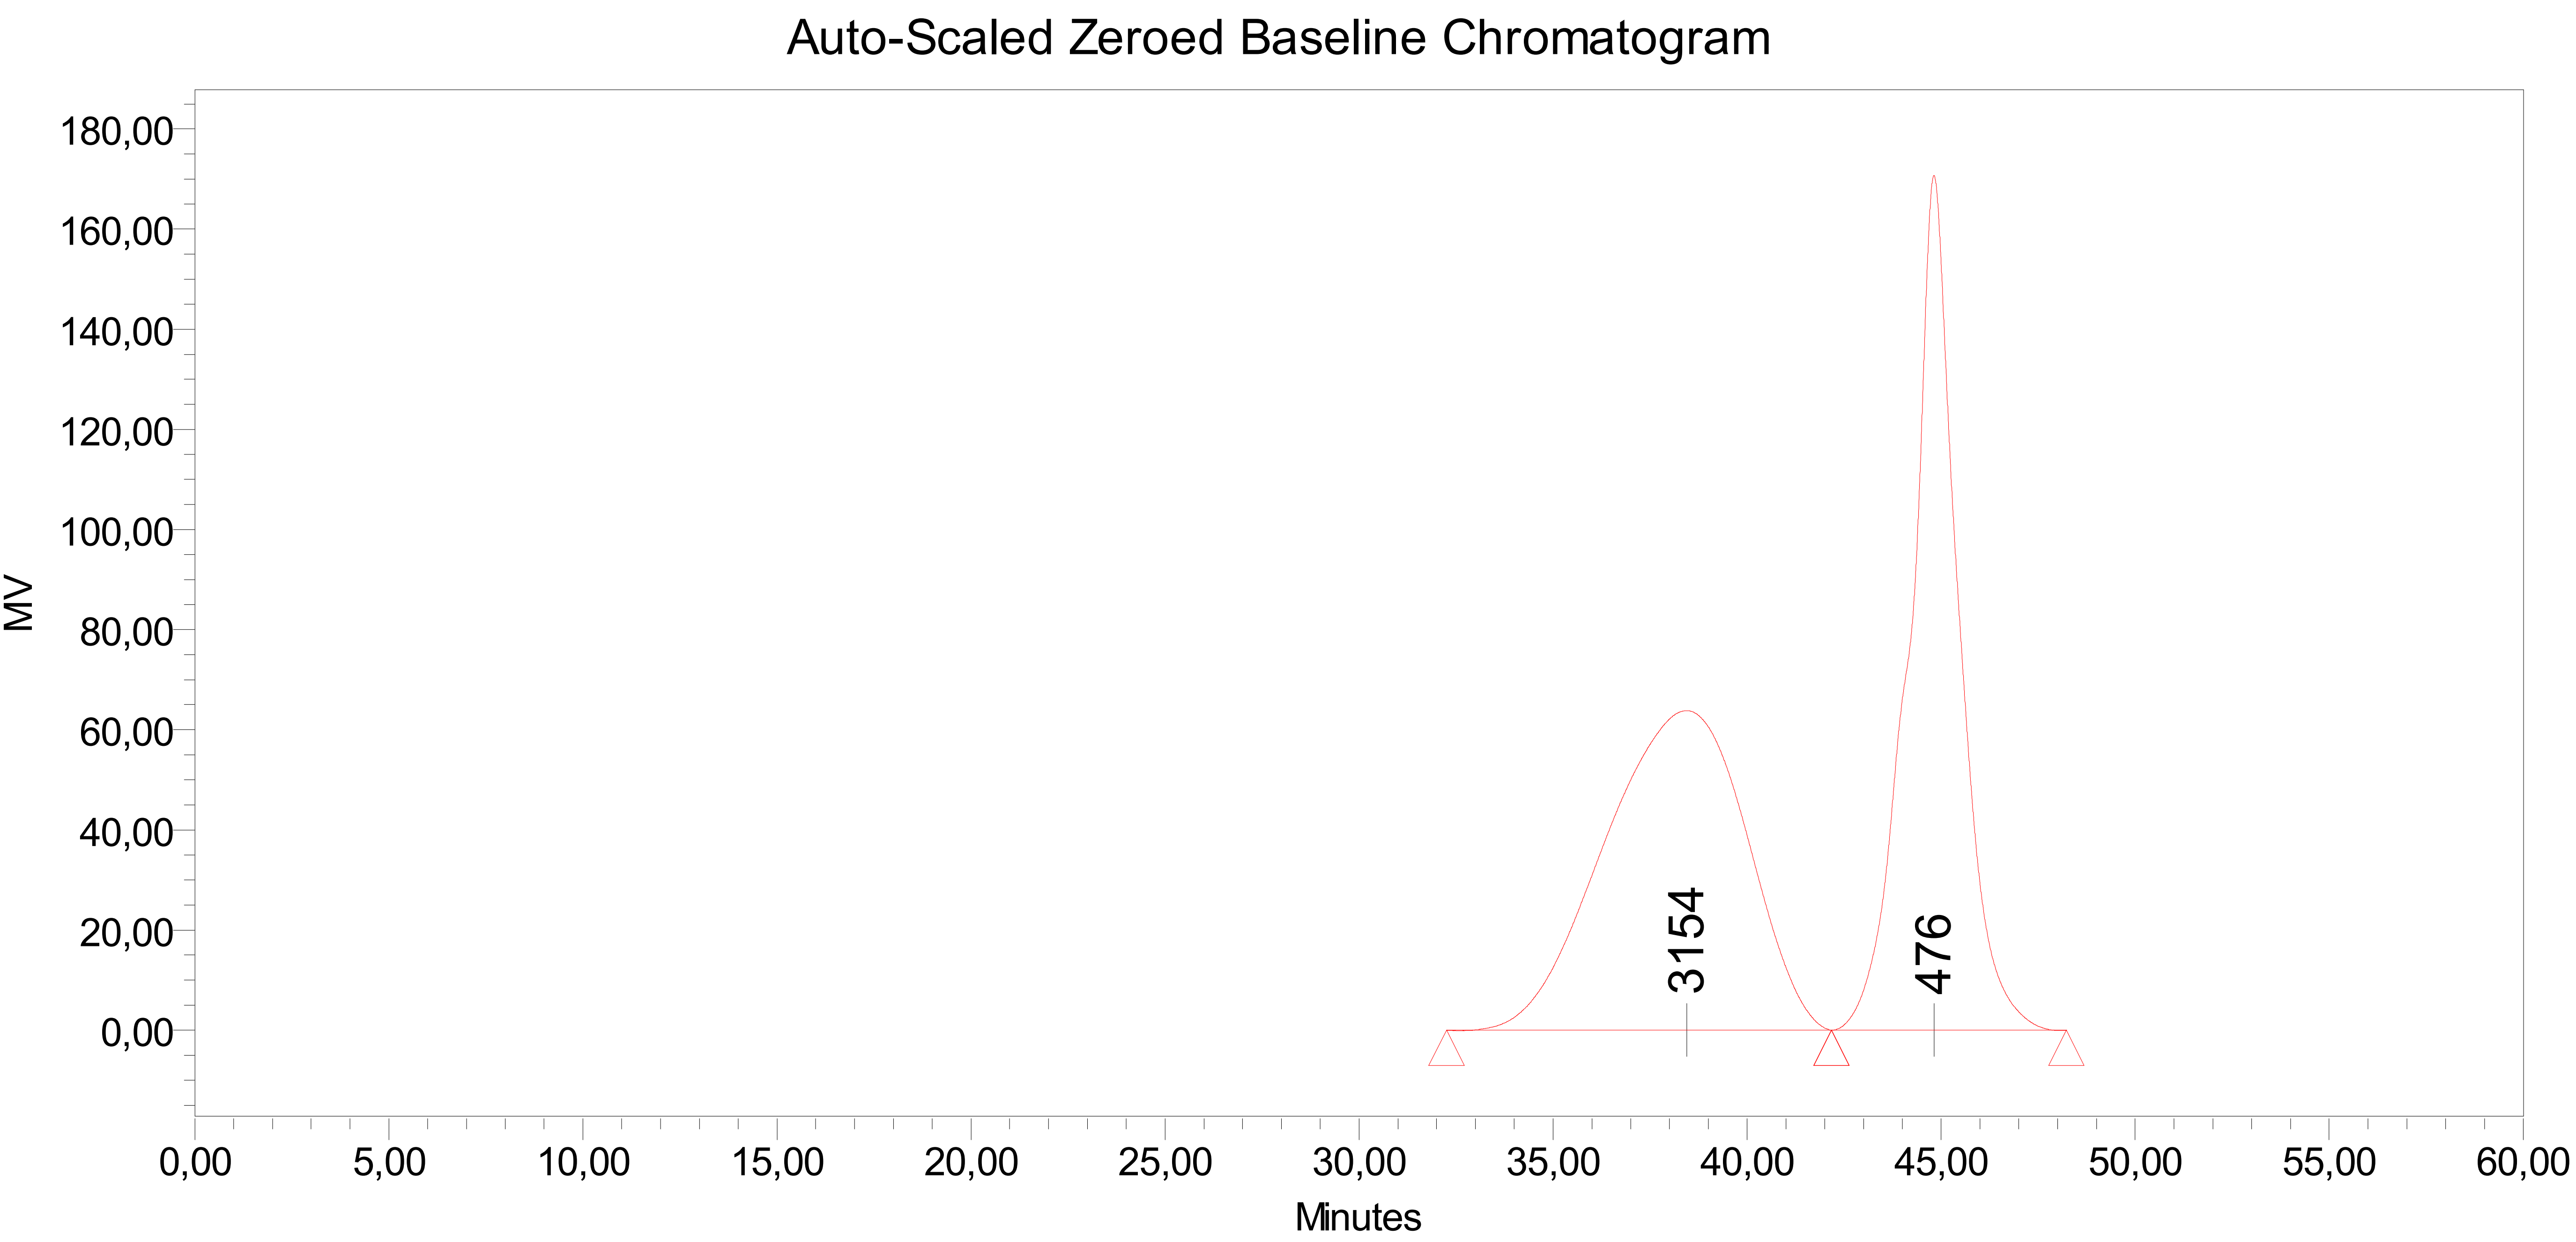

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	38,449	3199	4028	3154	5146	1,259	52,02
2	44,815	465	487	476	511	1,049	47,98

GPC Calibration Plot

