


Sample information

Sample Name:	Probka_15_PWS	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP_170217
Vial:	3	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-02-17 12:07:05 CET		
Processed:	2017-02-17 15:03:13 CET		

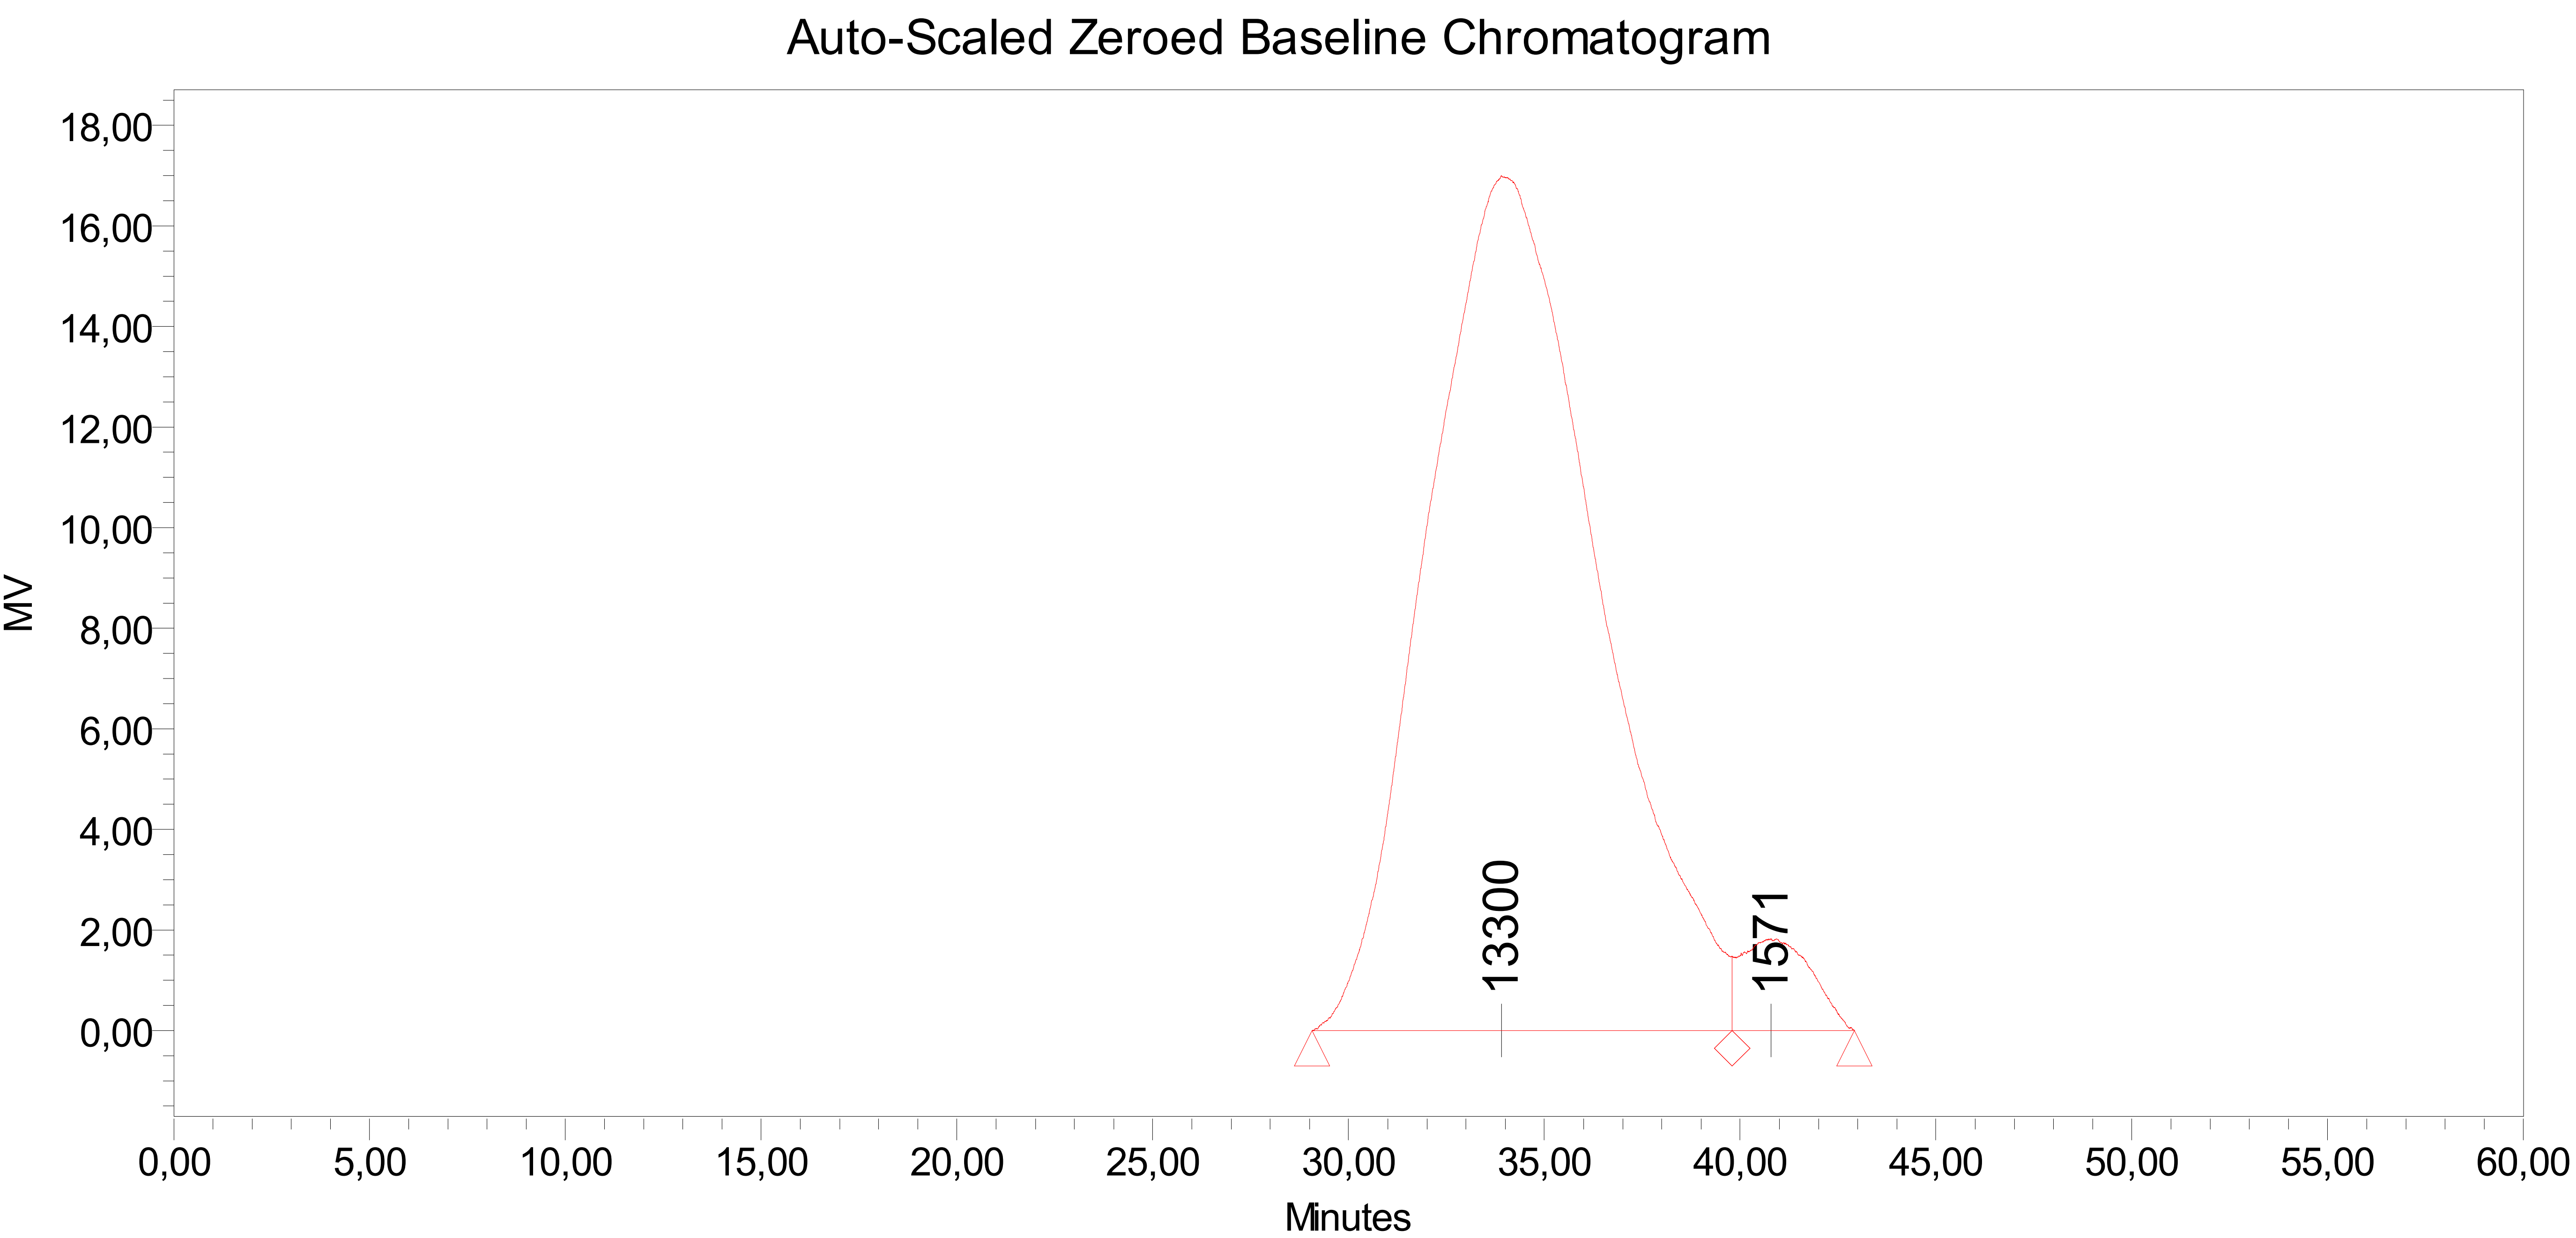

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	33,902	9136	14008	13300	21158	1,533	95,71
2	40,795	1444	1510	1571	1574	1,046	4,29

GPC Calibration Plot

