


Sample information

Sample Name:	Probka_4	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP_150317
Vial:	4	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-03-15 15:22:26 CET		
Processed:	2017-03-25 12:32:56 CET		

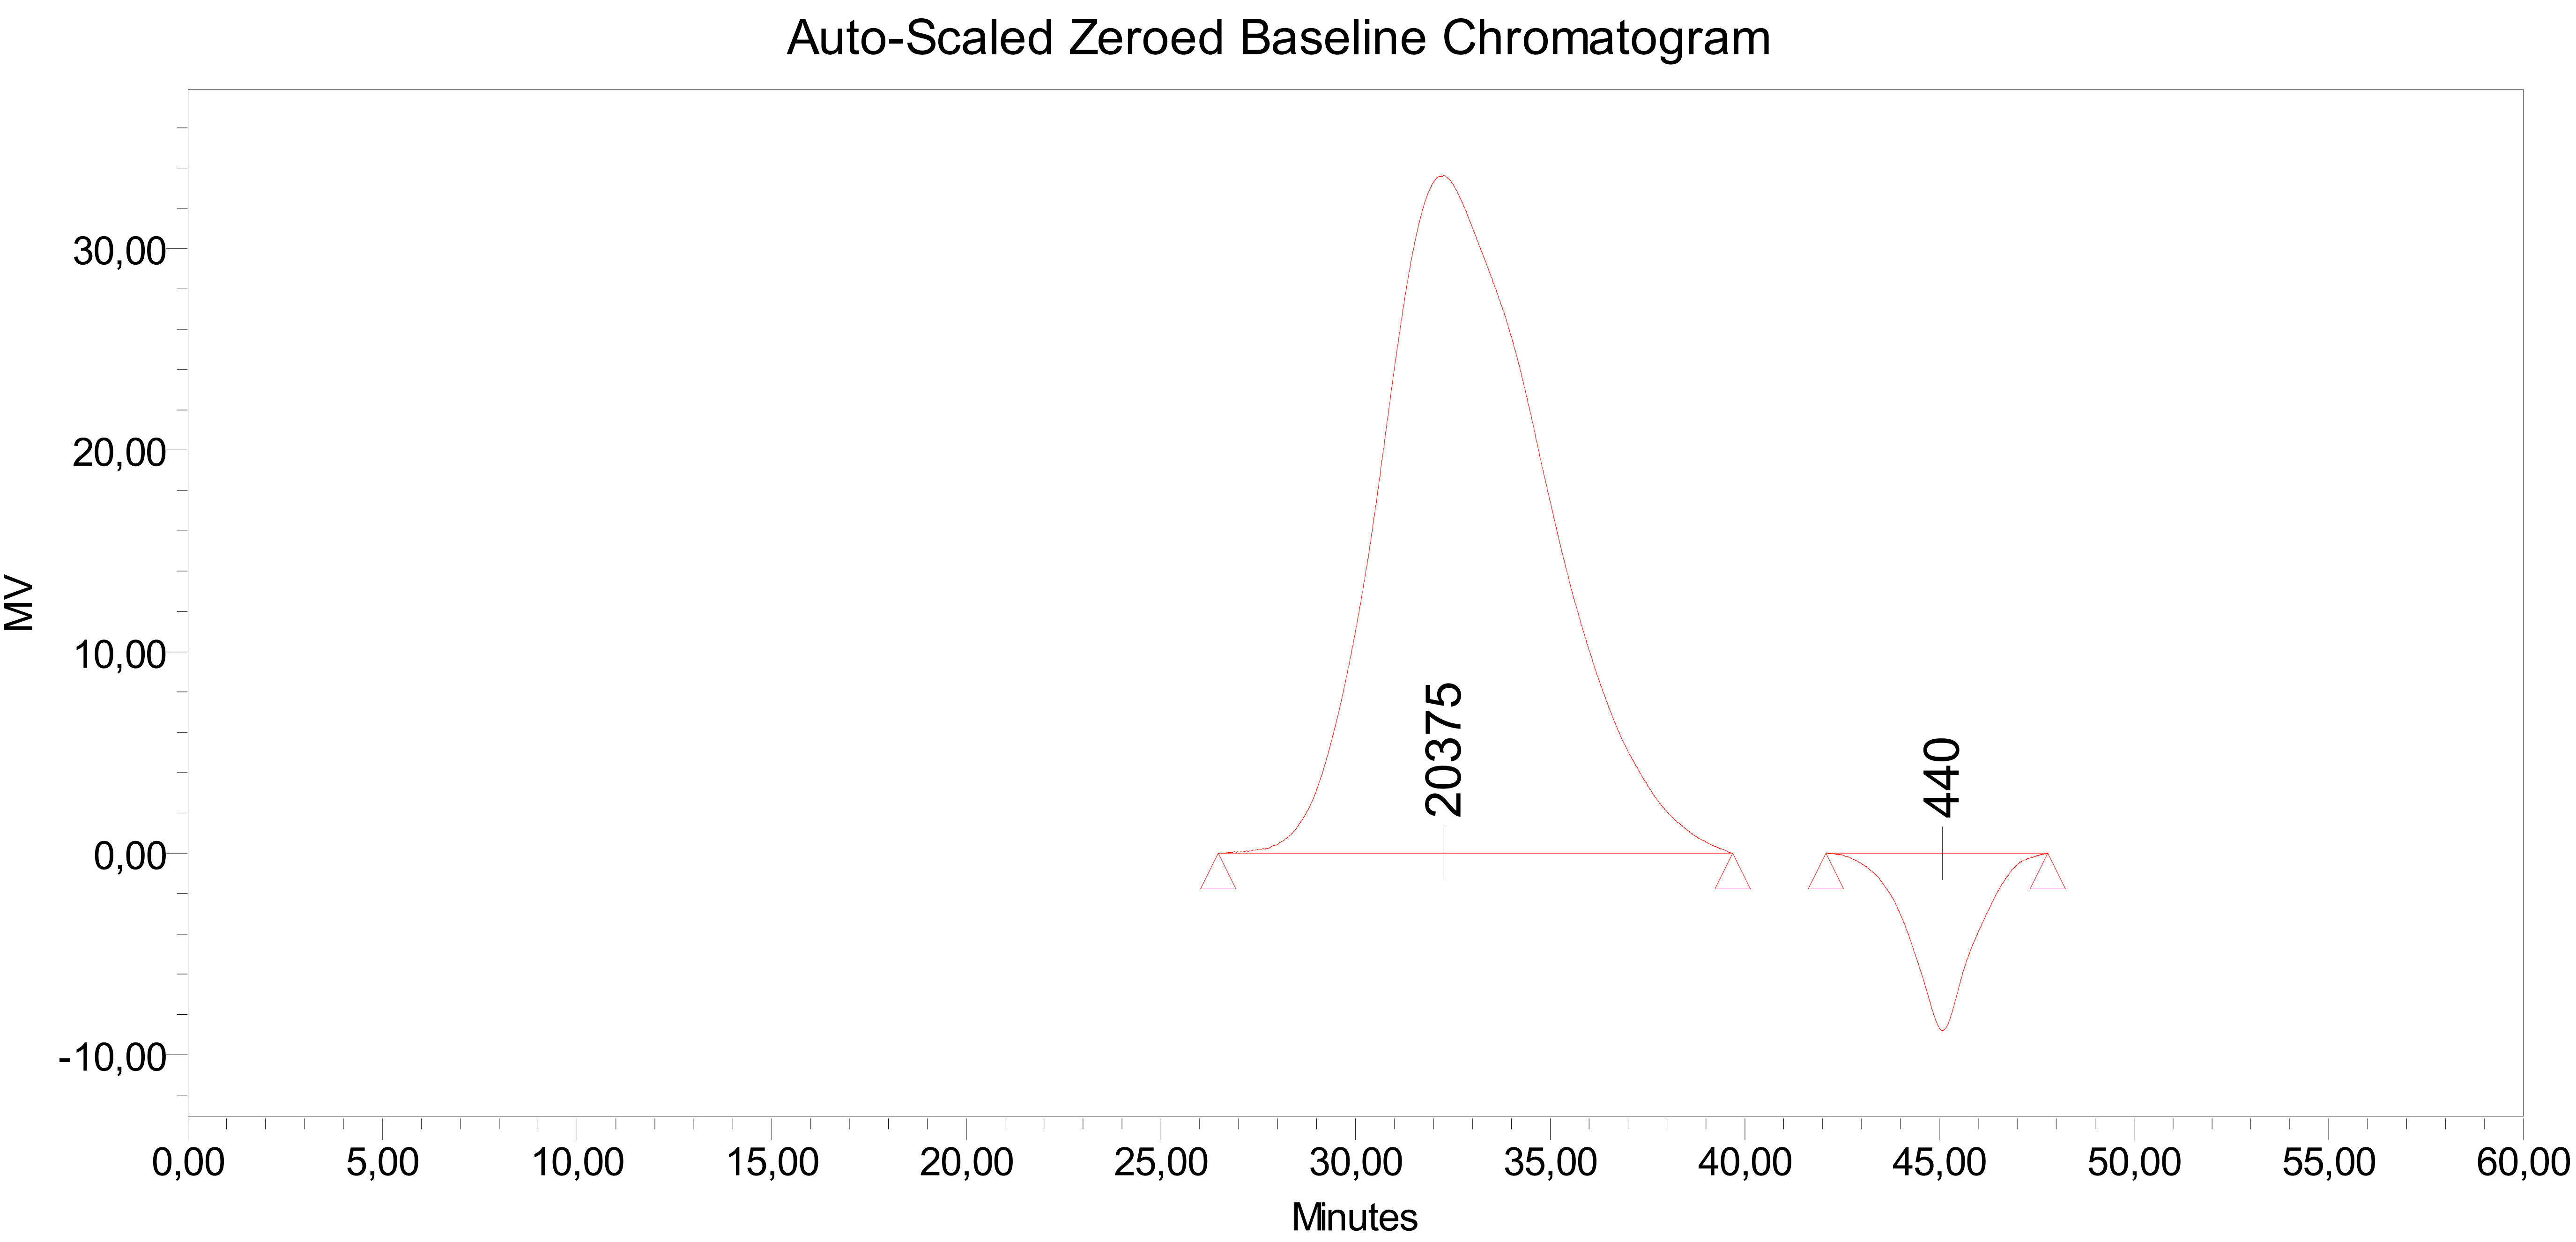

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	32,277	14617	24498	20375	45040	1,676	90,97
2	45,081	428	455	440	485	1,064	9,03

GPC Calibration Plot

