


Sample information

Sample Name:	Probka_2	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP_150317
Vial:	2	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-03-15 13:20:49 CET		
Processed:	2017-03-25 12:32:07 CET		

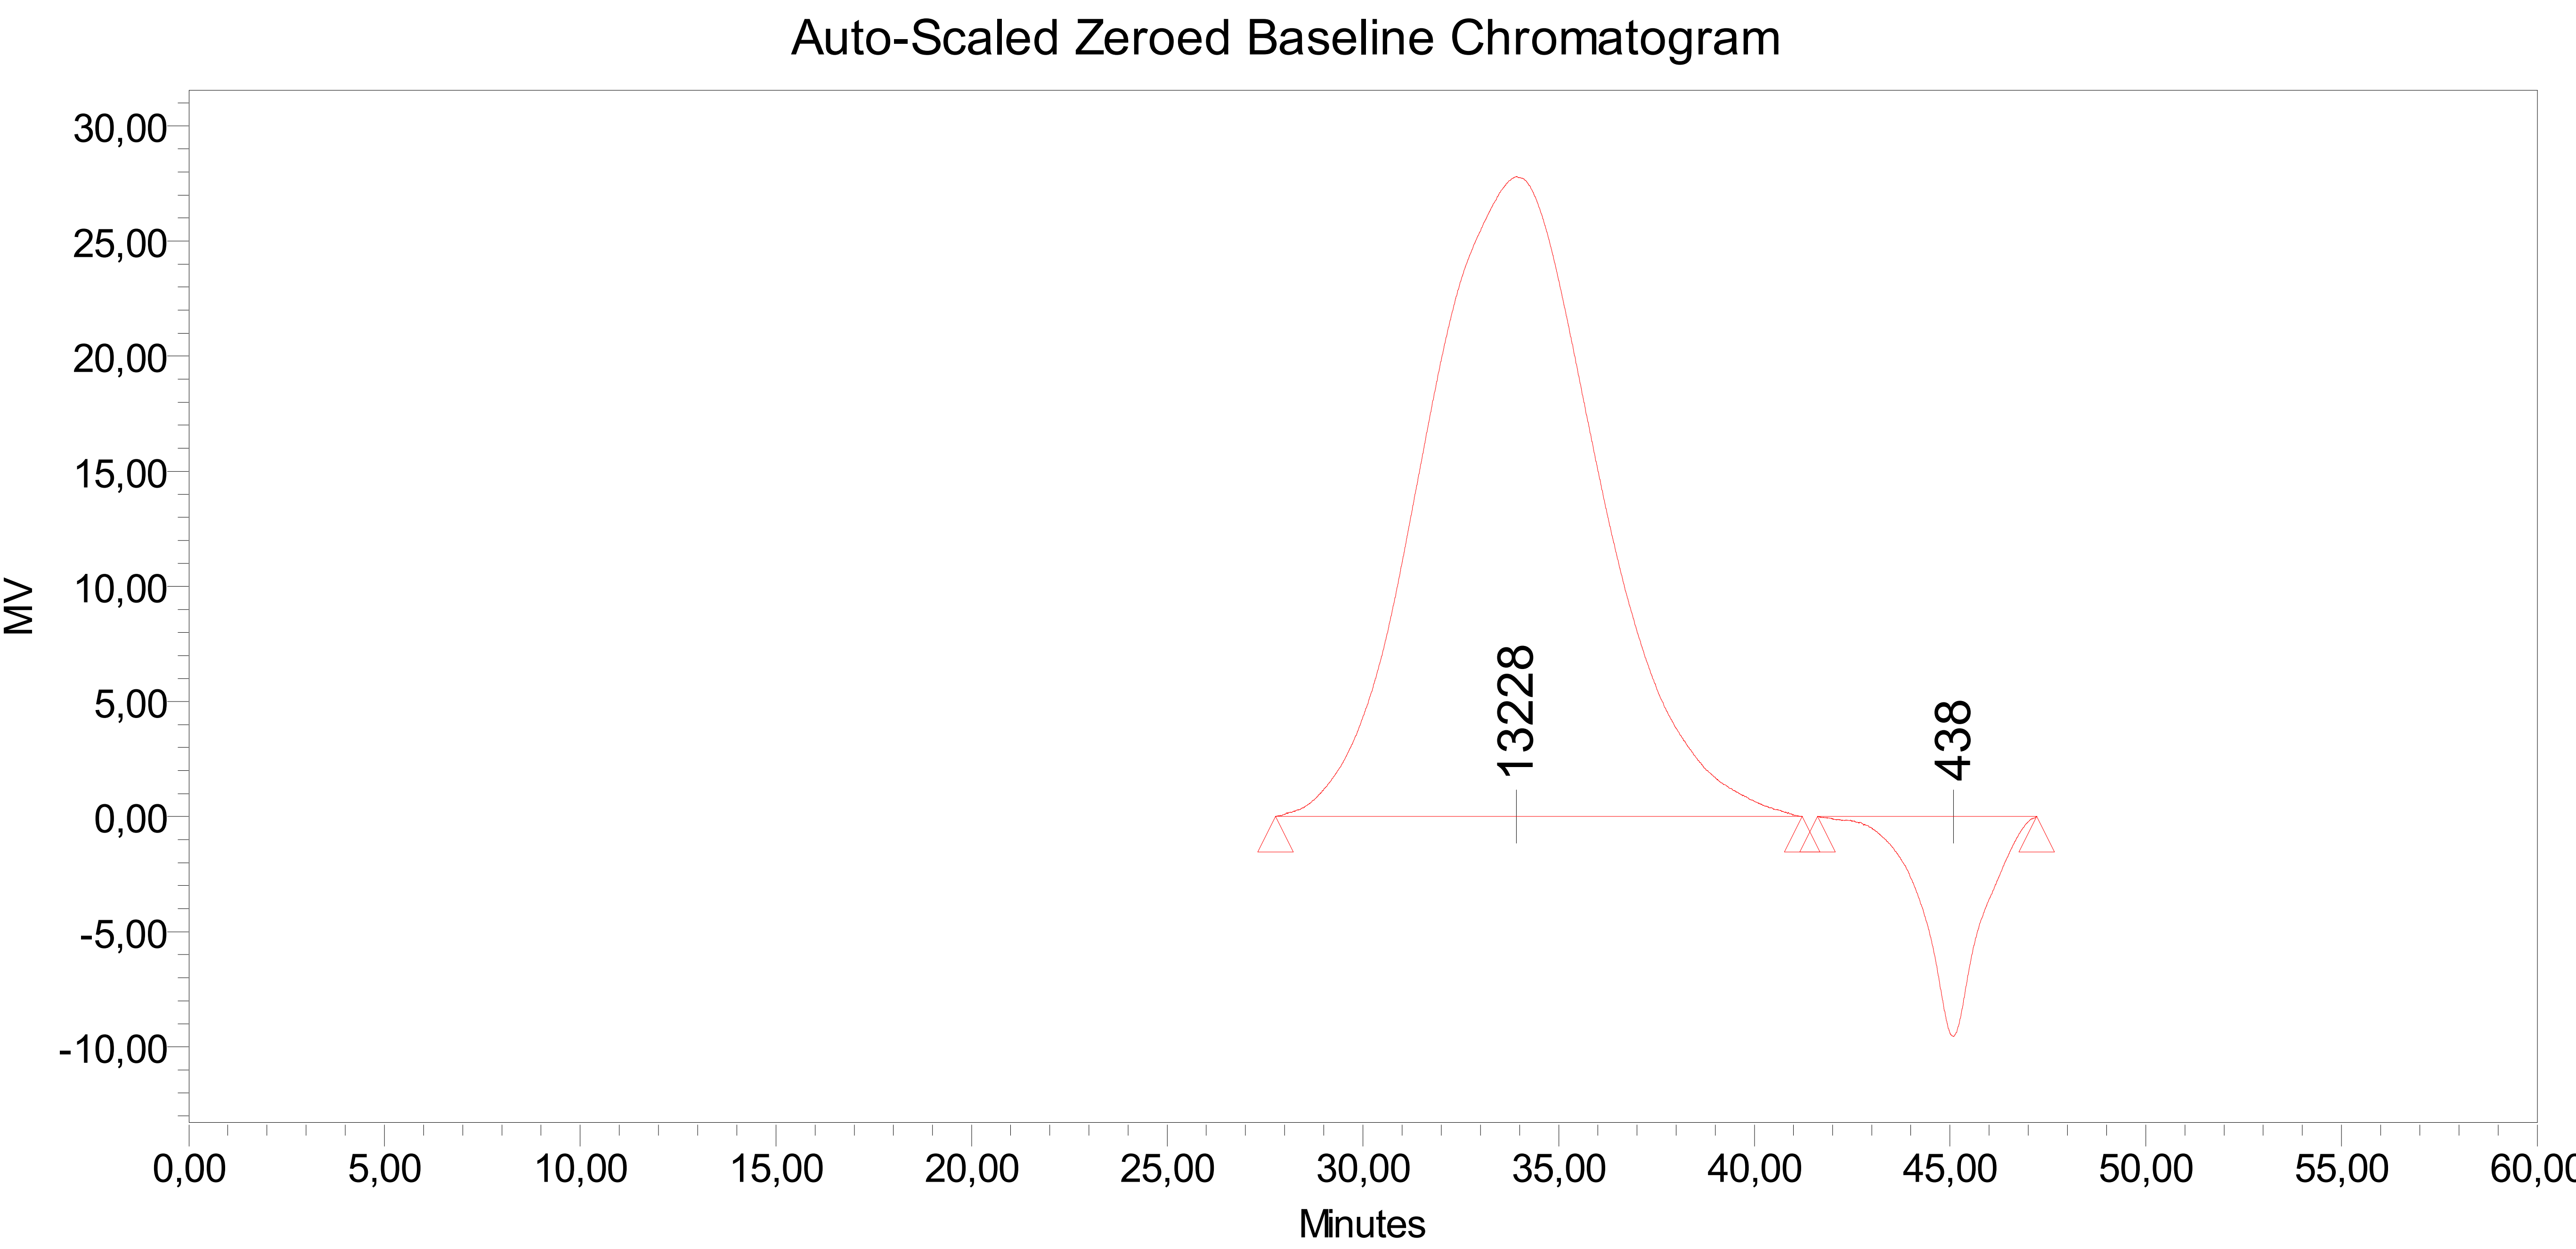

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	33,919	10698	17481	13228	31231	1,634	90,10
2	45,093	435	461	438	492	1,060	9,90

GPC Calibration Plot

