


Sample information

Sample Name:	crosslinker210	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	sip250716
Vial:	5	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_sip
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2016-07-25 16:52:39 CEST		
Processed:	2016-07-25 20:16:05 CEST		

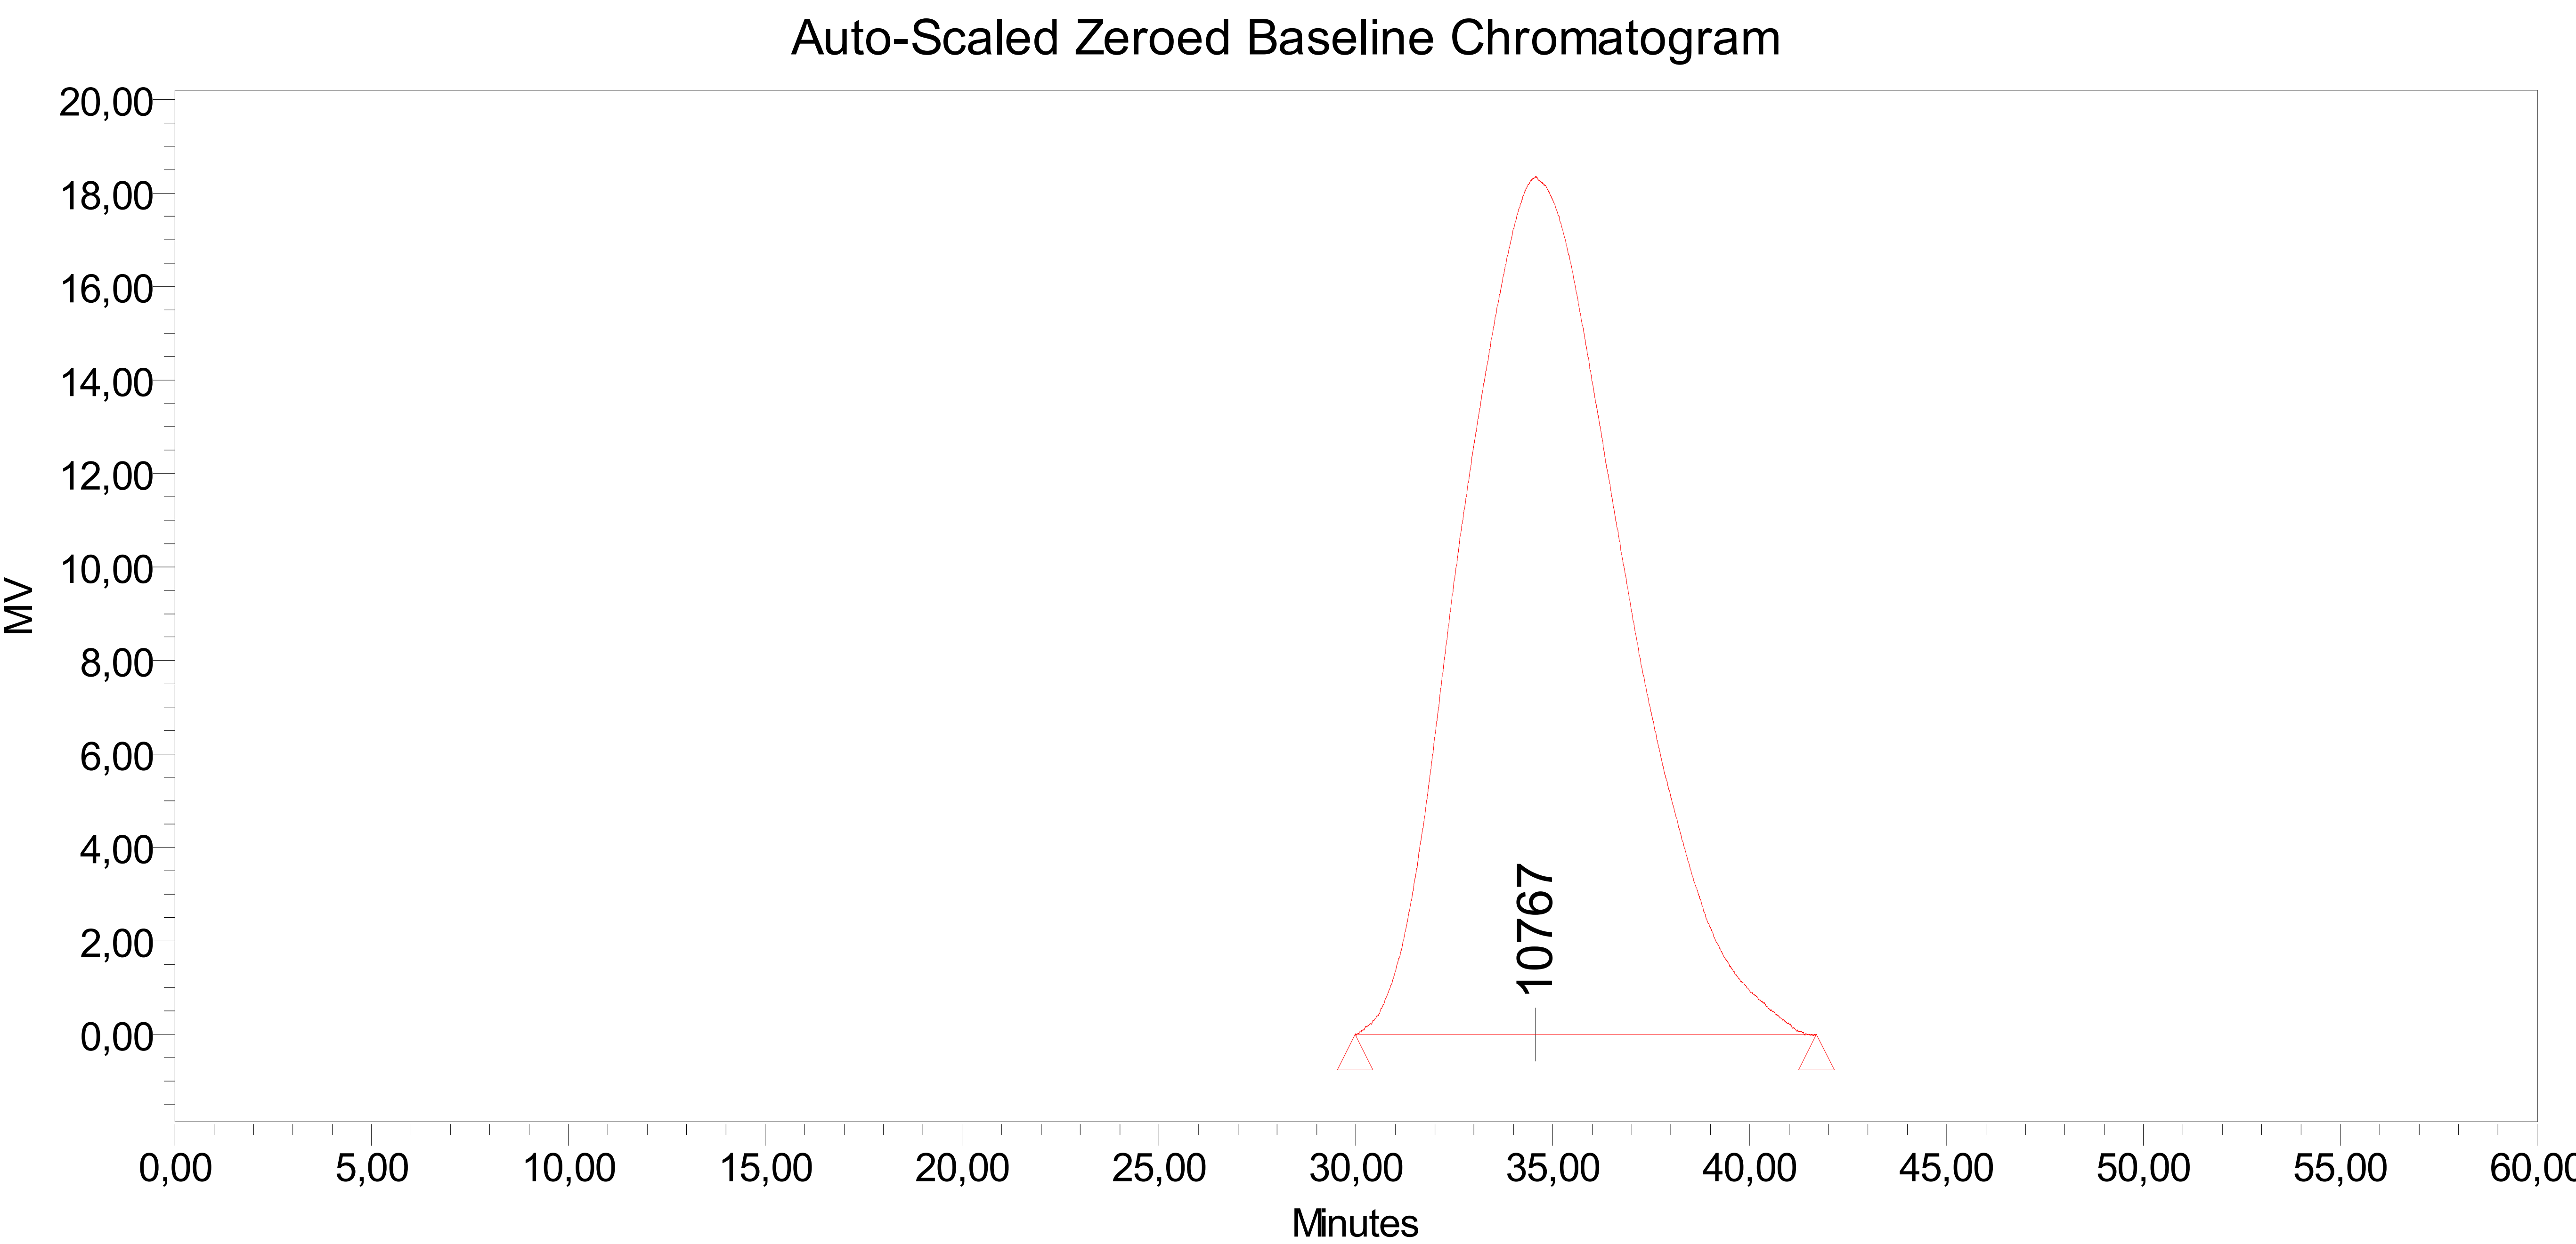

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	34,562	7863	11185	10767	15144	1,422	100,00

GPC Calibration Plot

