


Sample information

Sample Name:	Probka_13_PVS	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP_170217
Vial:	1	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-02-17 10:05:26 CET		
Processed:	2017-02-17 15:01:41 CET		

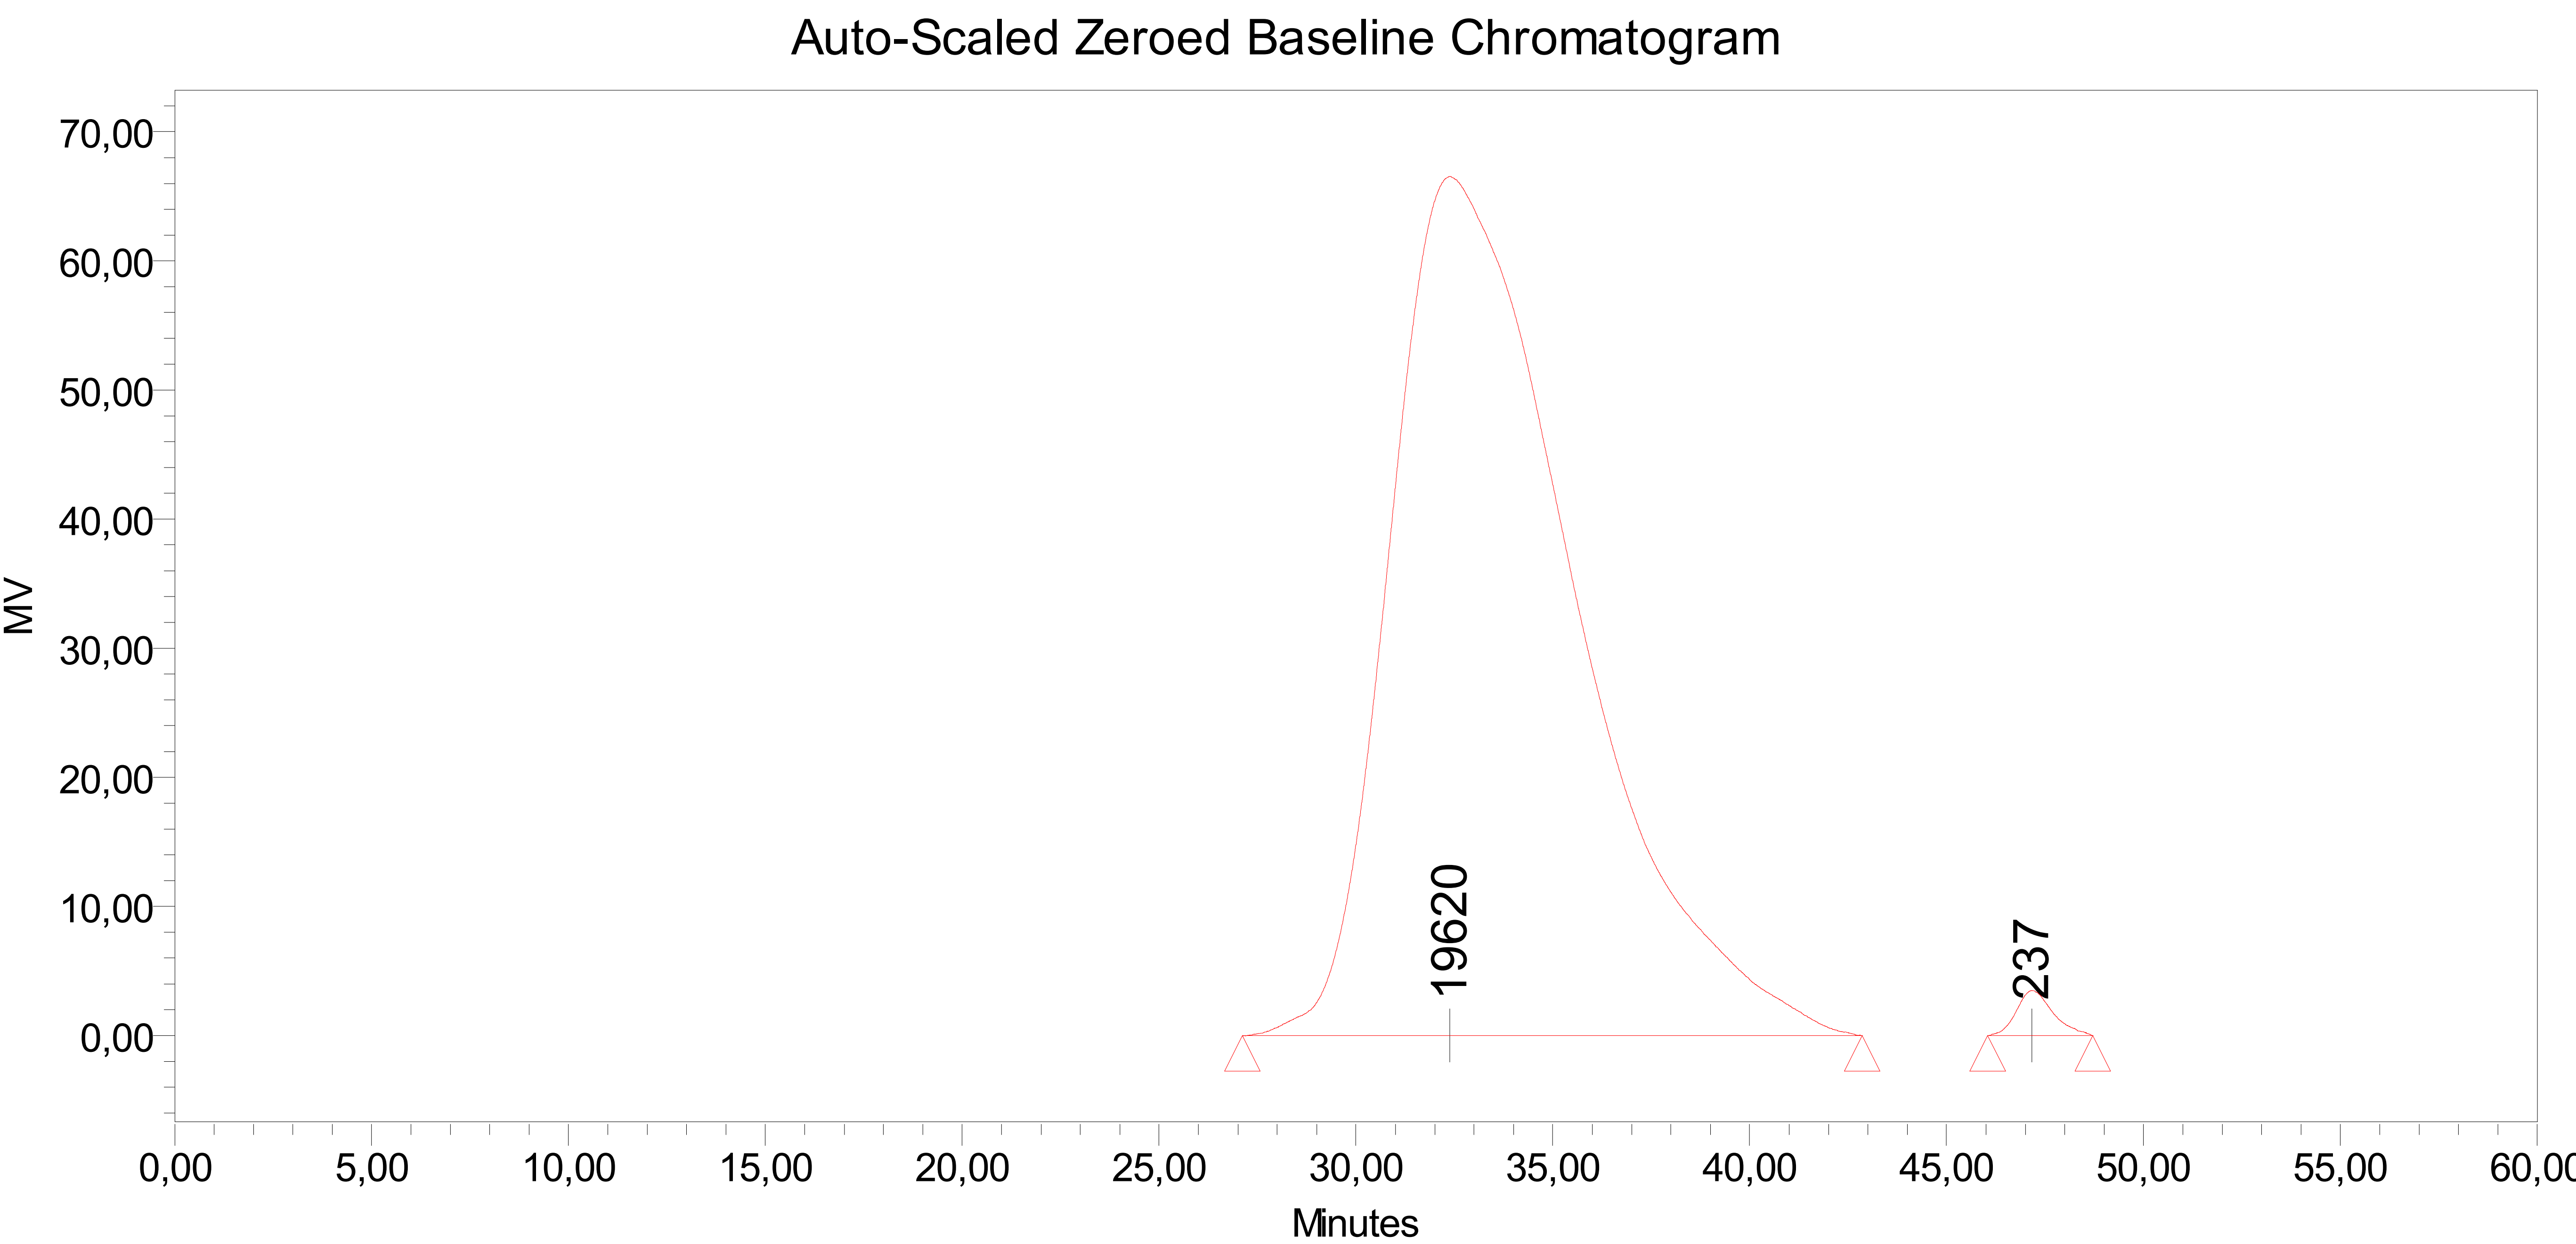

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	32,387	10360	19768	19620	35345	1,908	98,97
2	47,162	226	230	237	234	1,019	1,03

GPC Calibration Plot

