


Sample information

Sample Name:	Probka_35	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP021017
Vial:	8	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-10-02 17:35:28 CEST		
Processed:	2017-10-03 09:29:36 CEST		

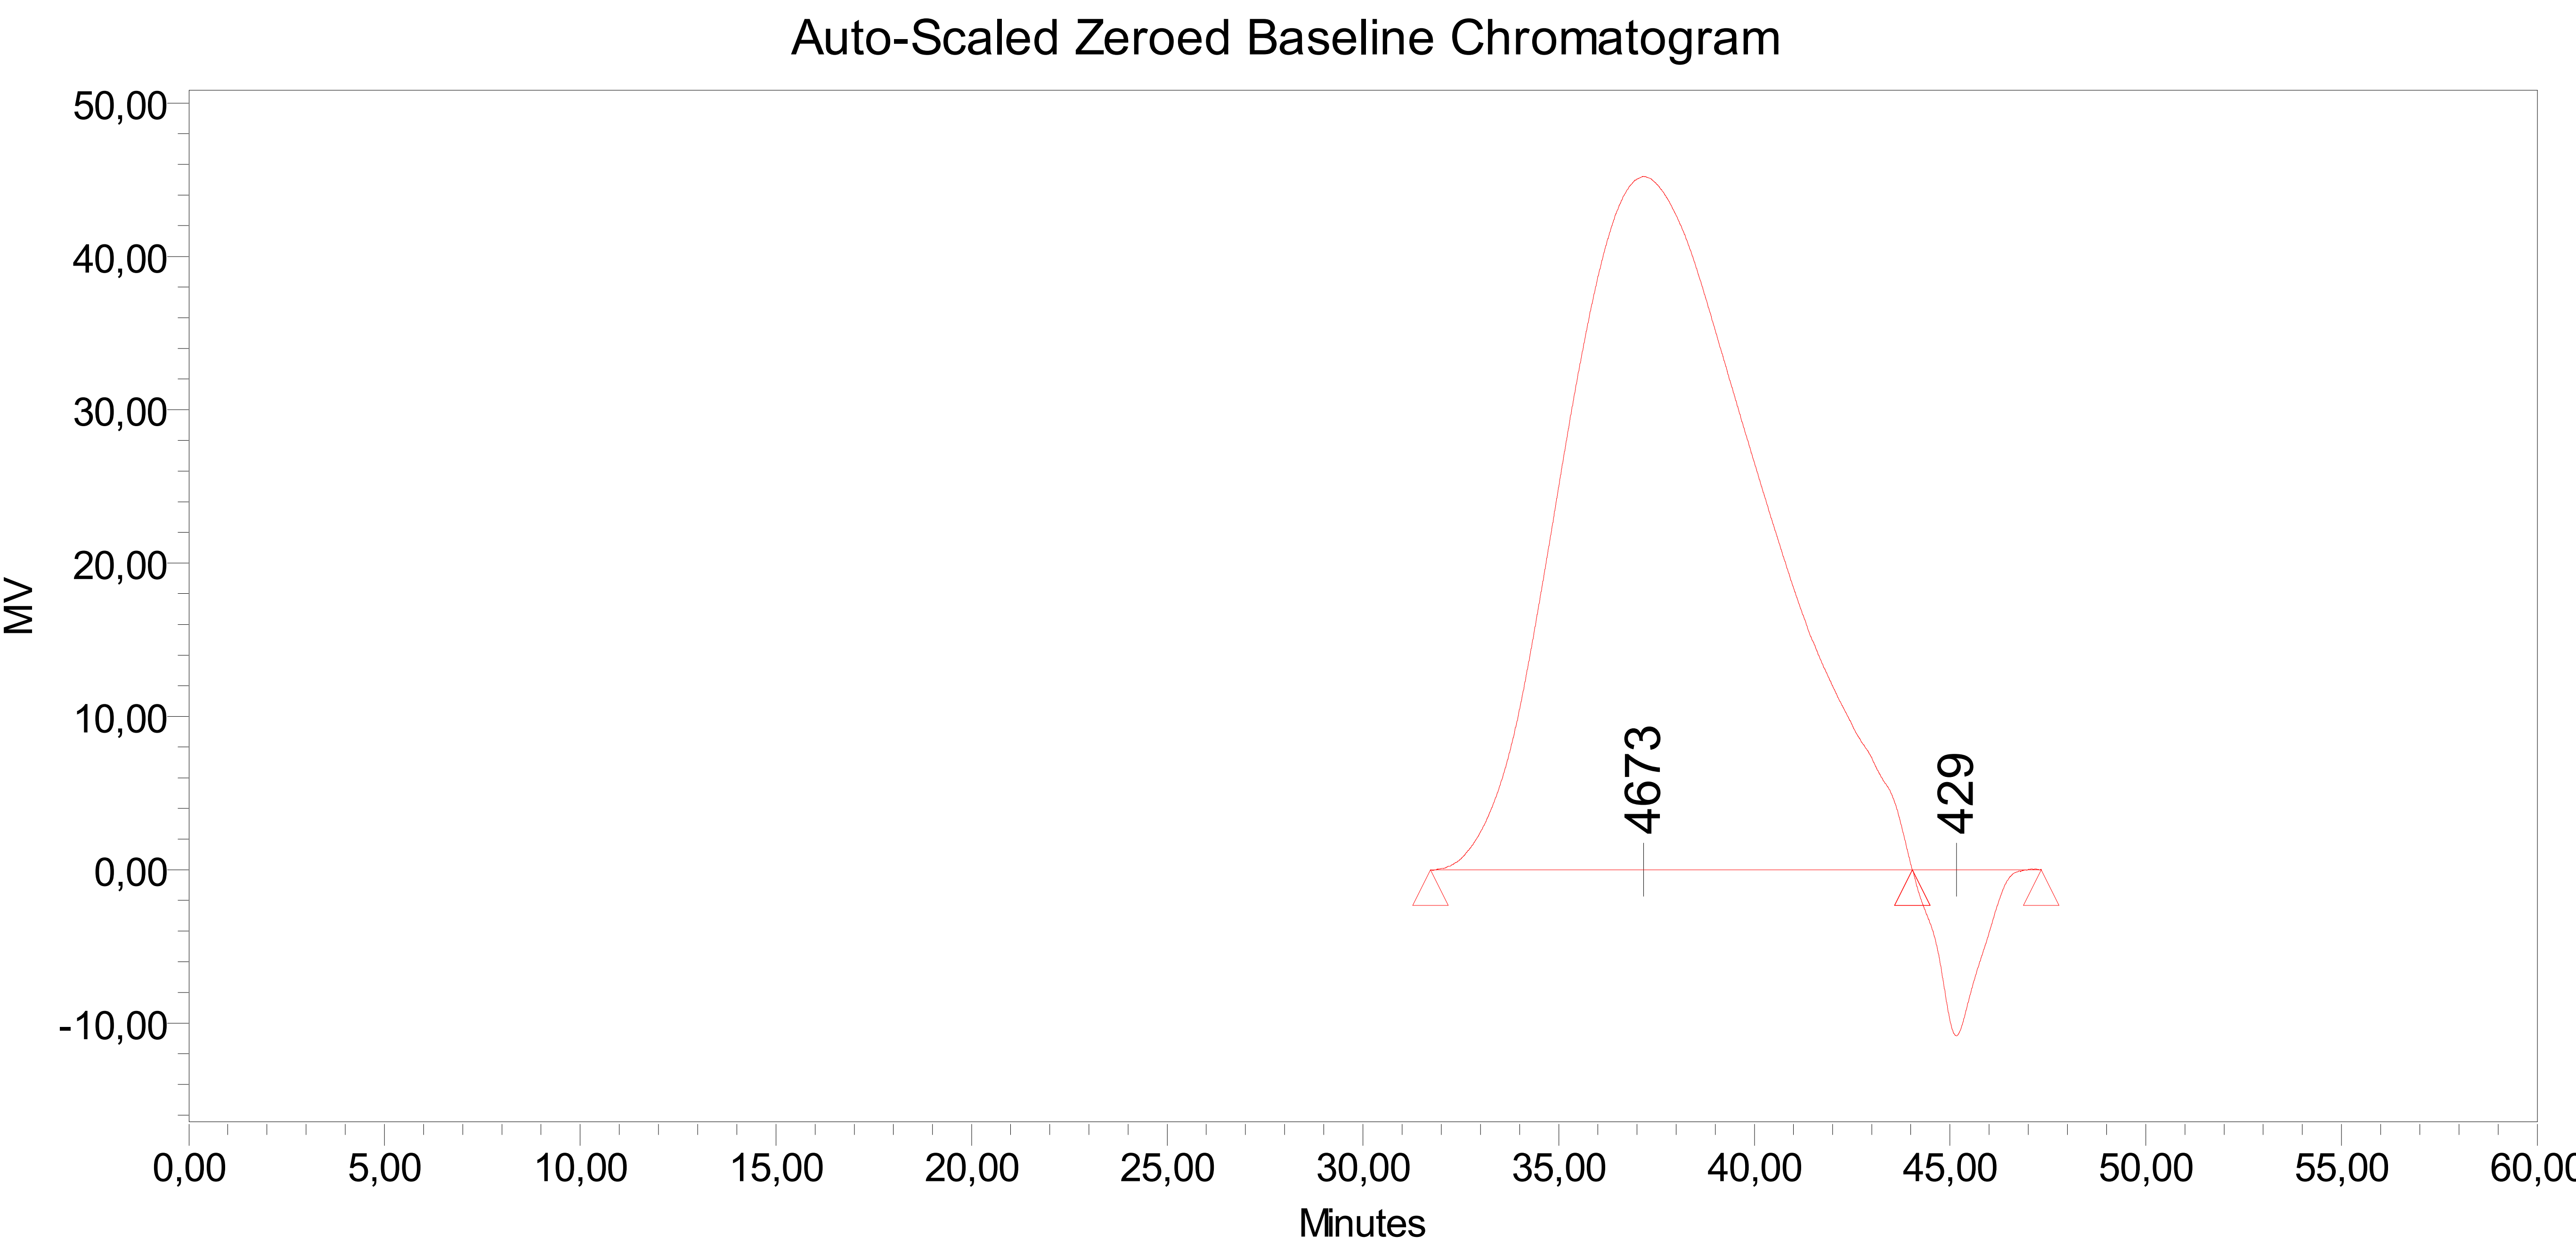

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	37,167	2913	4695	4673	6837	1,612	95,23
2	45,166	411	421	429	430	1,023	4,77

GPC Calibration Plot

