


Sample information

Sample Name:	crosslinker125	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	sip250716
Vial:	3	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_sip
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2016-07-25 14:51:01 CEST		
Processed:	2016-07-25 20:15:15 CEST		

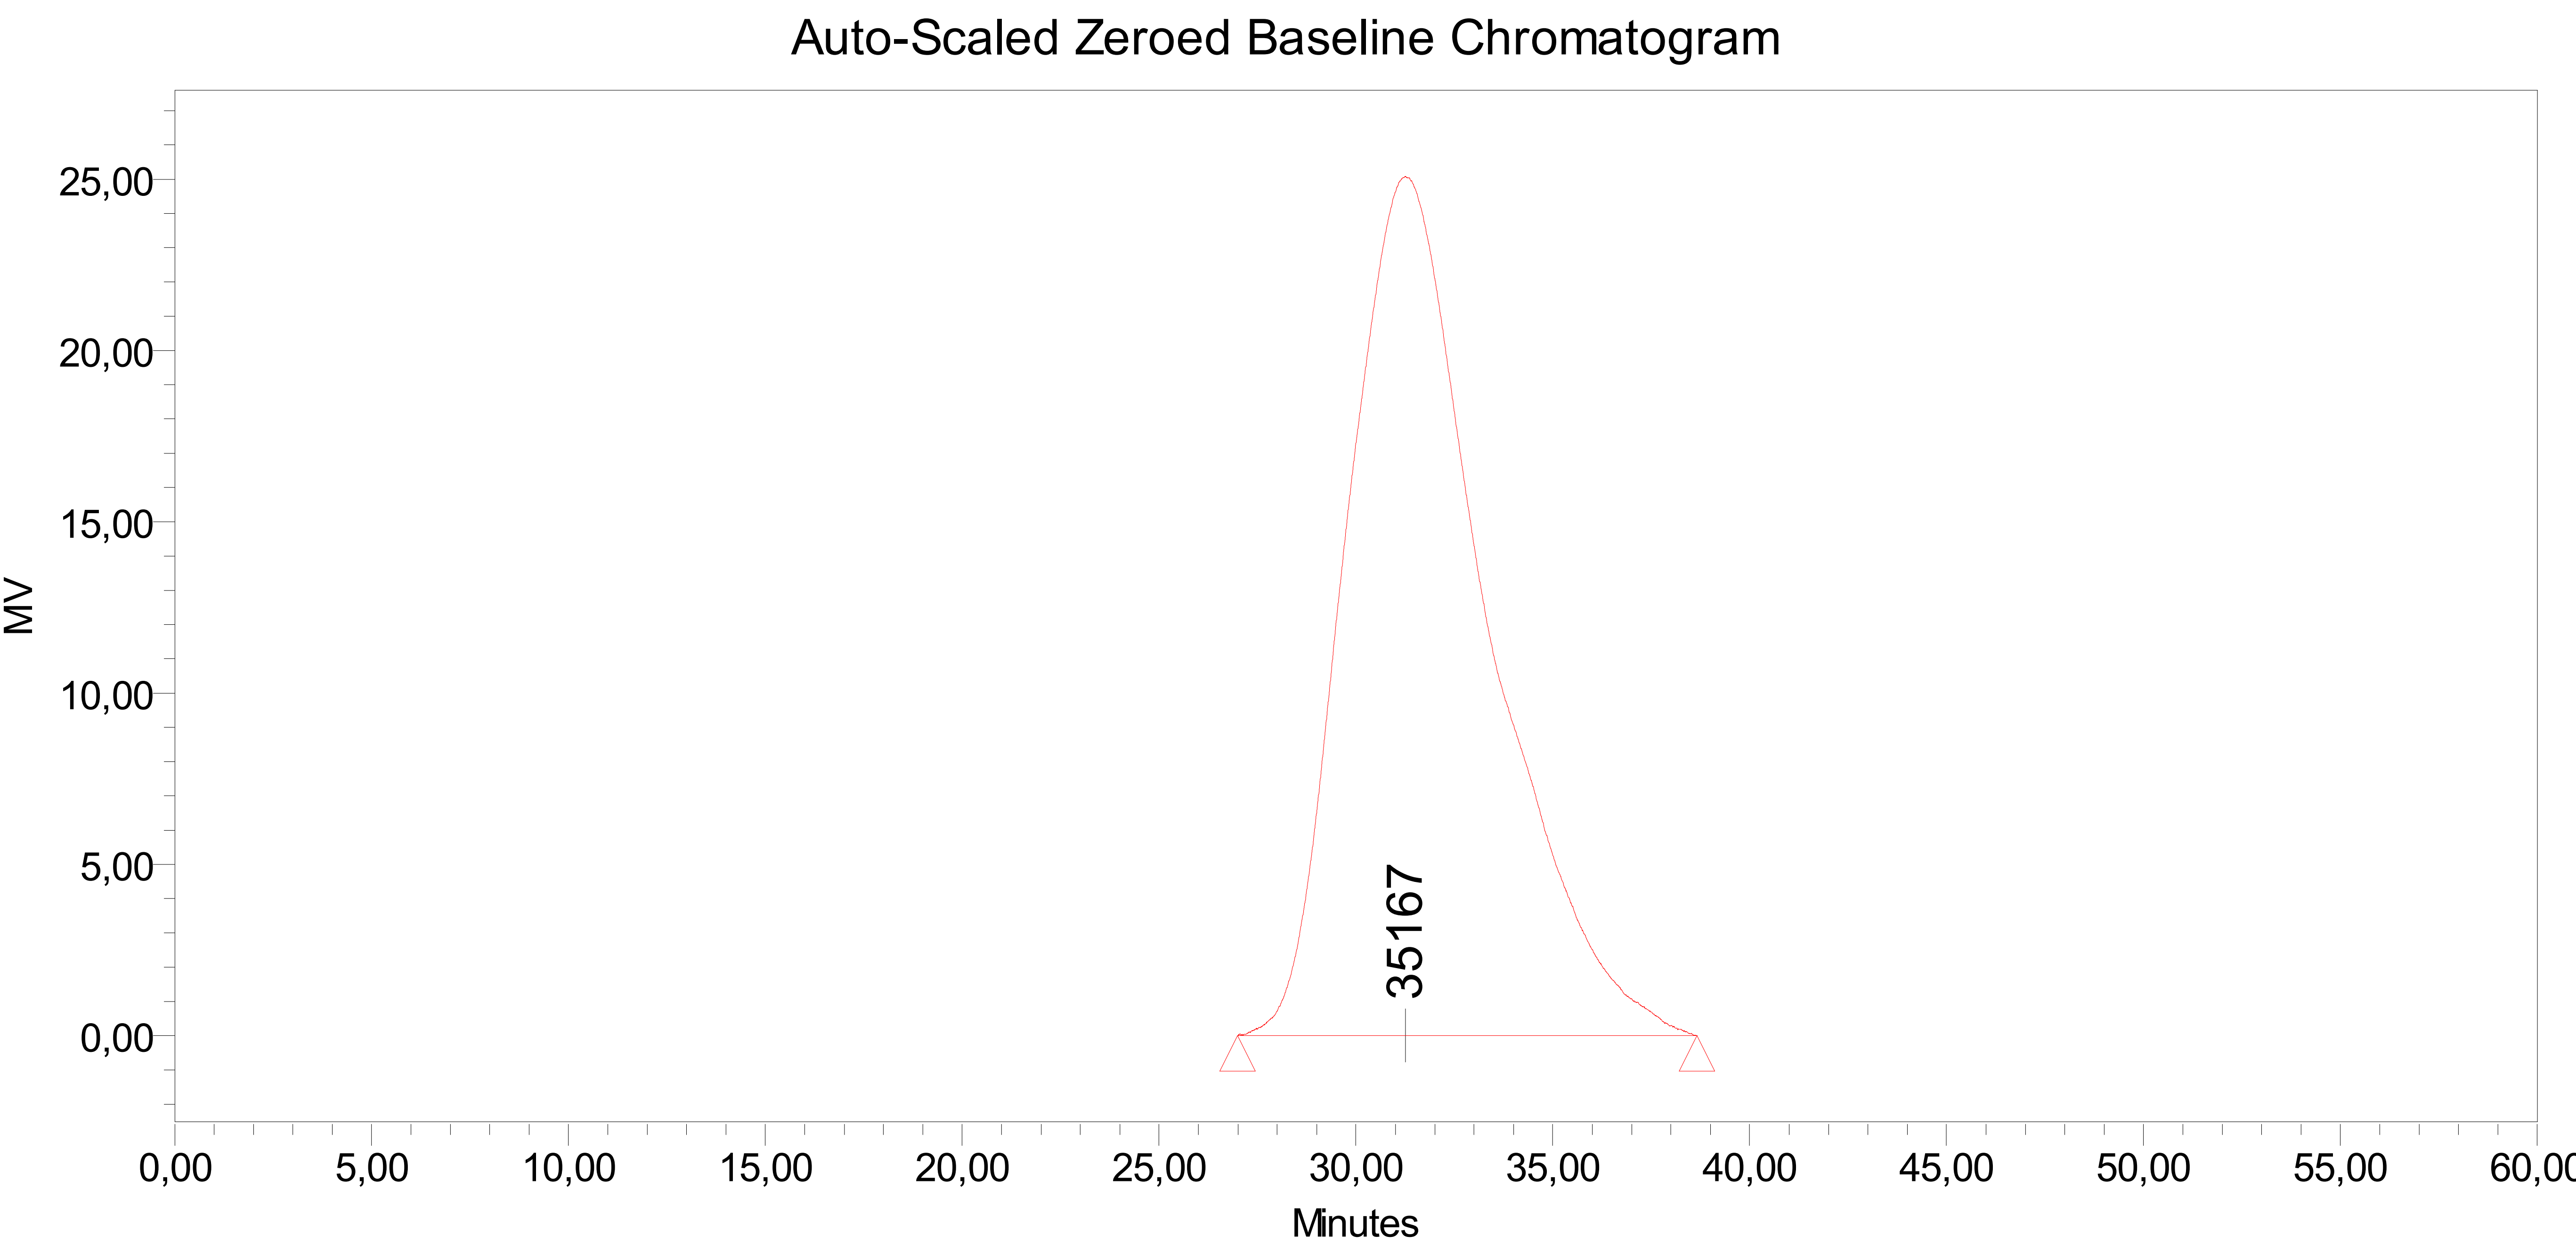

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	31,250	22174	37518	35167	61031	1,692	100,00

GPC Calibration Plot

