


Sample information

Sample Name:	SiP_pr42	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	011217
Vial:	1	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_MD
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-12-01 09:36:29 CET		
Processed:	2017-12-01 15:36:59 CET		

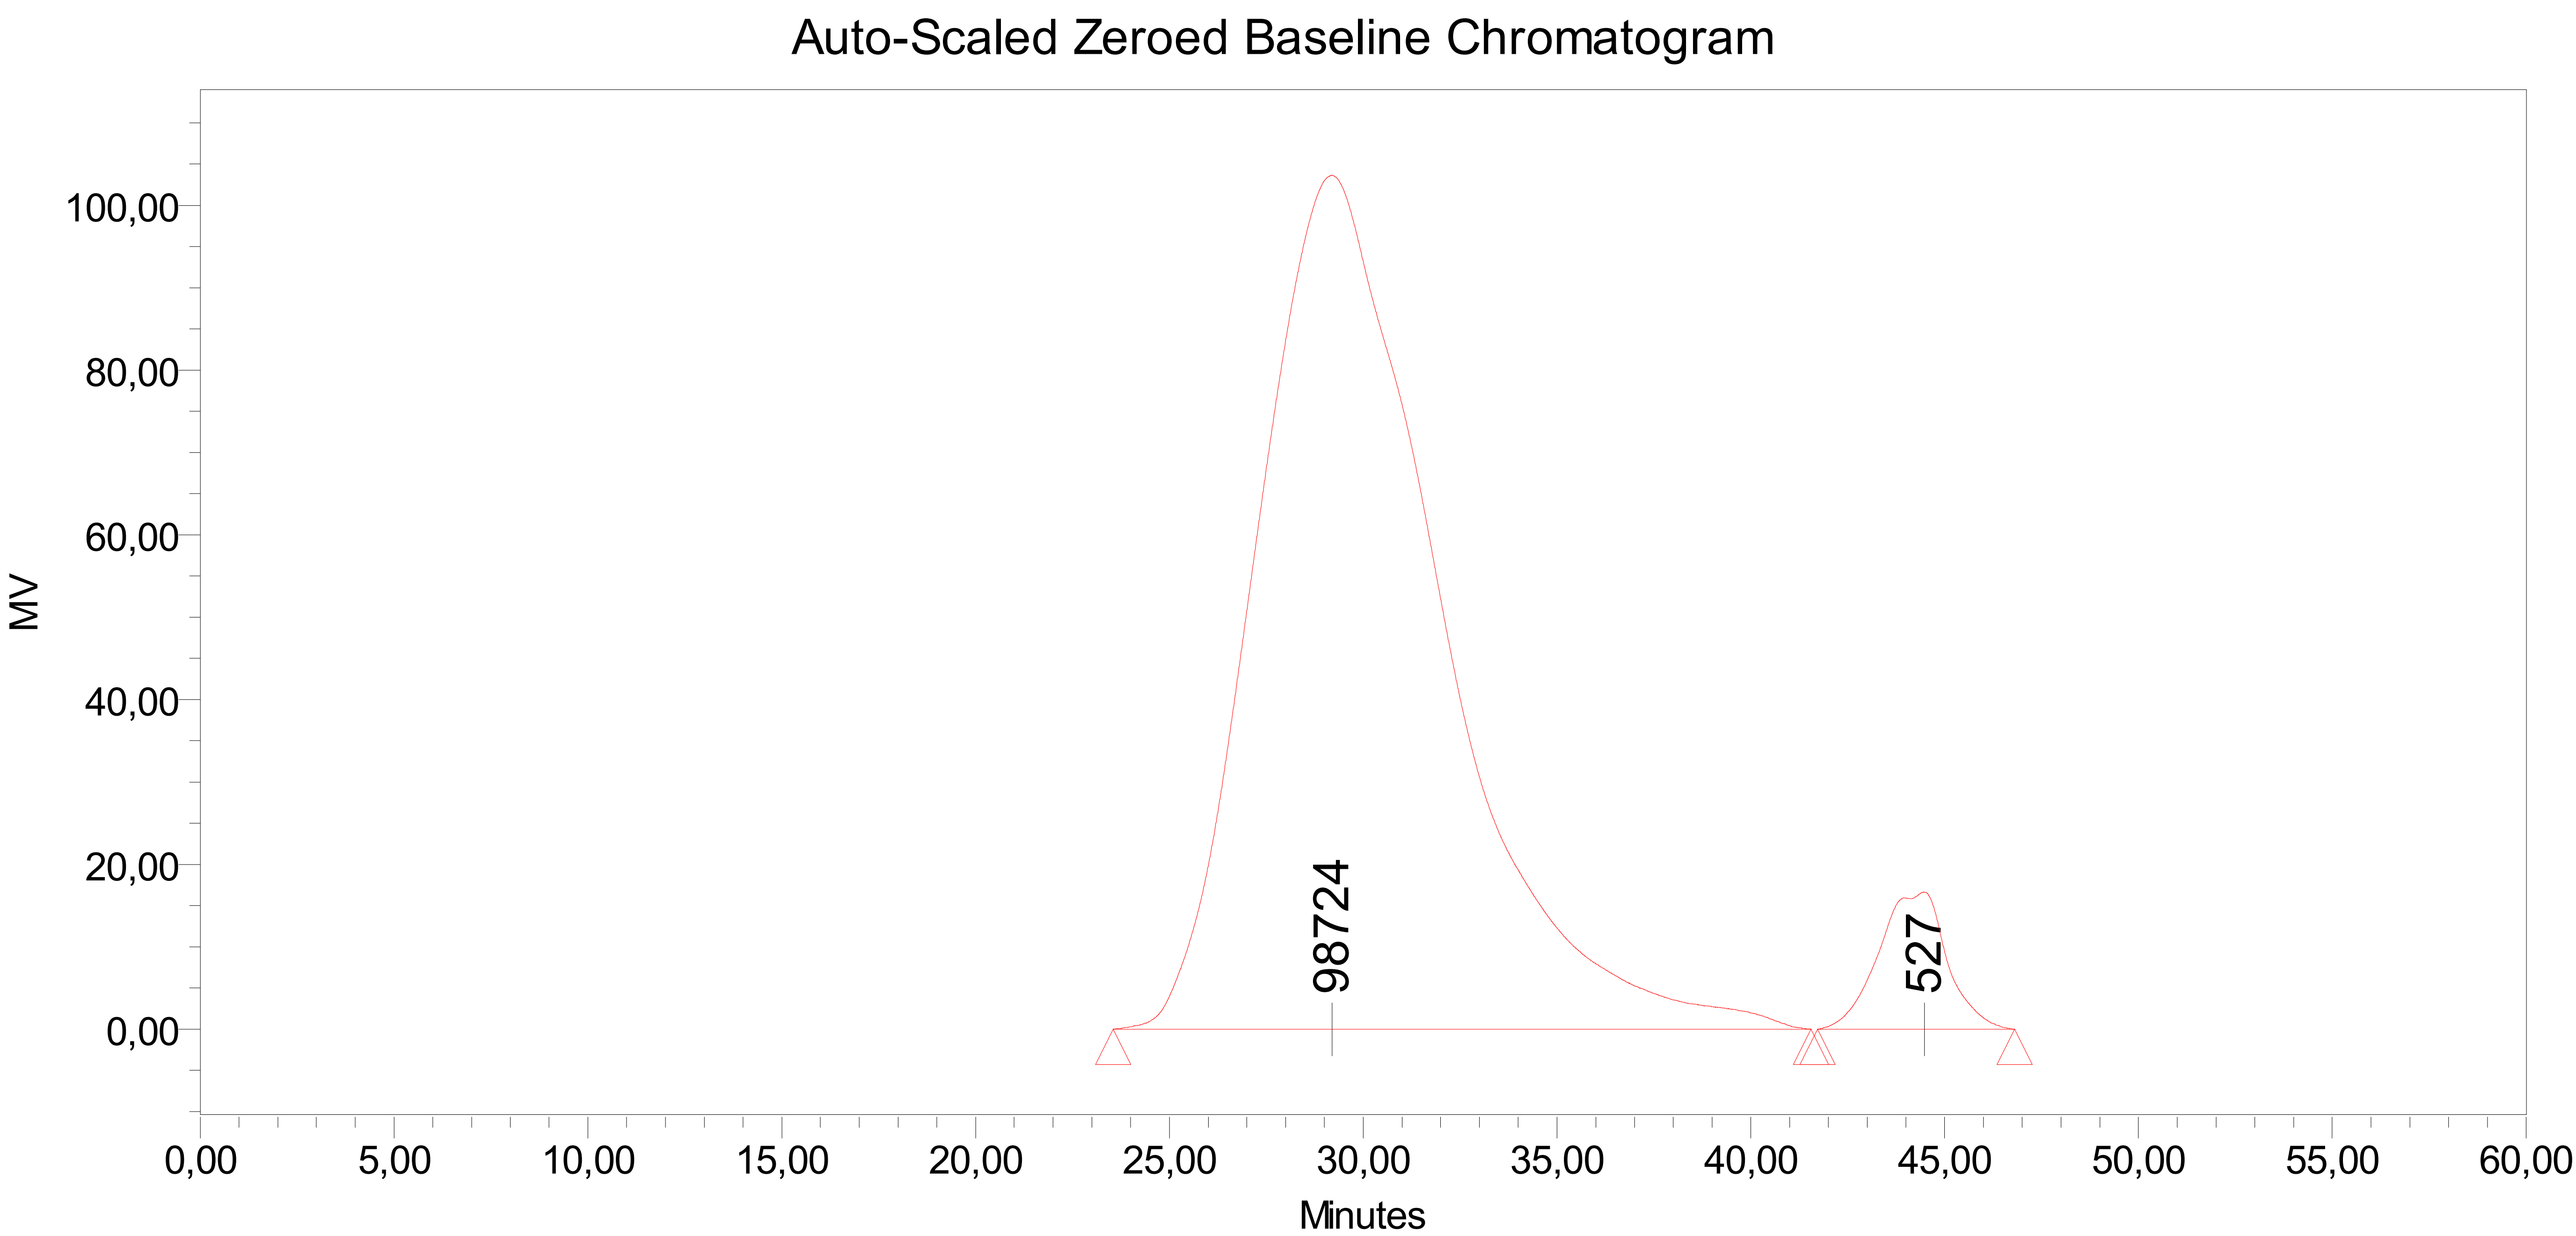

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	29,198	32795	151133	98724	550889	4,608	94,36
2	44,474	562	593	527	626	1,056	5,64

GPC Calibration Plot

