


Sample information

Sample Name:	Probka_23	Acquired By:	System
Sample Type:	Broad Unknown	Sample Set Name:	SiP_010817
Vial:	5	Acq. Method Set:	standardowa THF
Injection #:	1	Proc. Method:	thf_06_ptp_md
Inj. Volume:	10,00 ul	Channel Name:	410
Run Time:	60,0 Minutes	Proc. Chnl. Descr.:	
Acquired:	2017-08-01 13:41:08 CEST		
Processed:	2017-08-24 17:26:35 CEST		

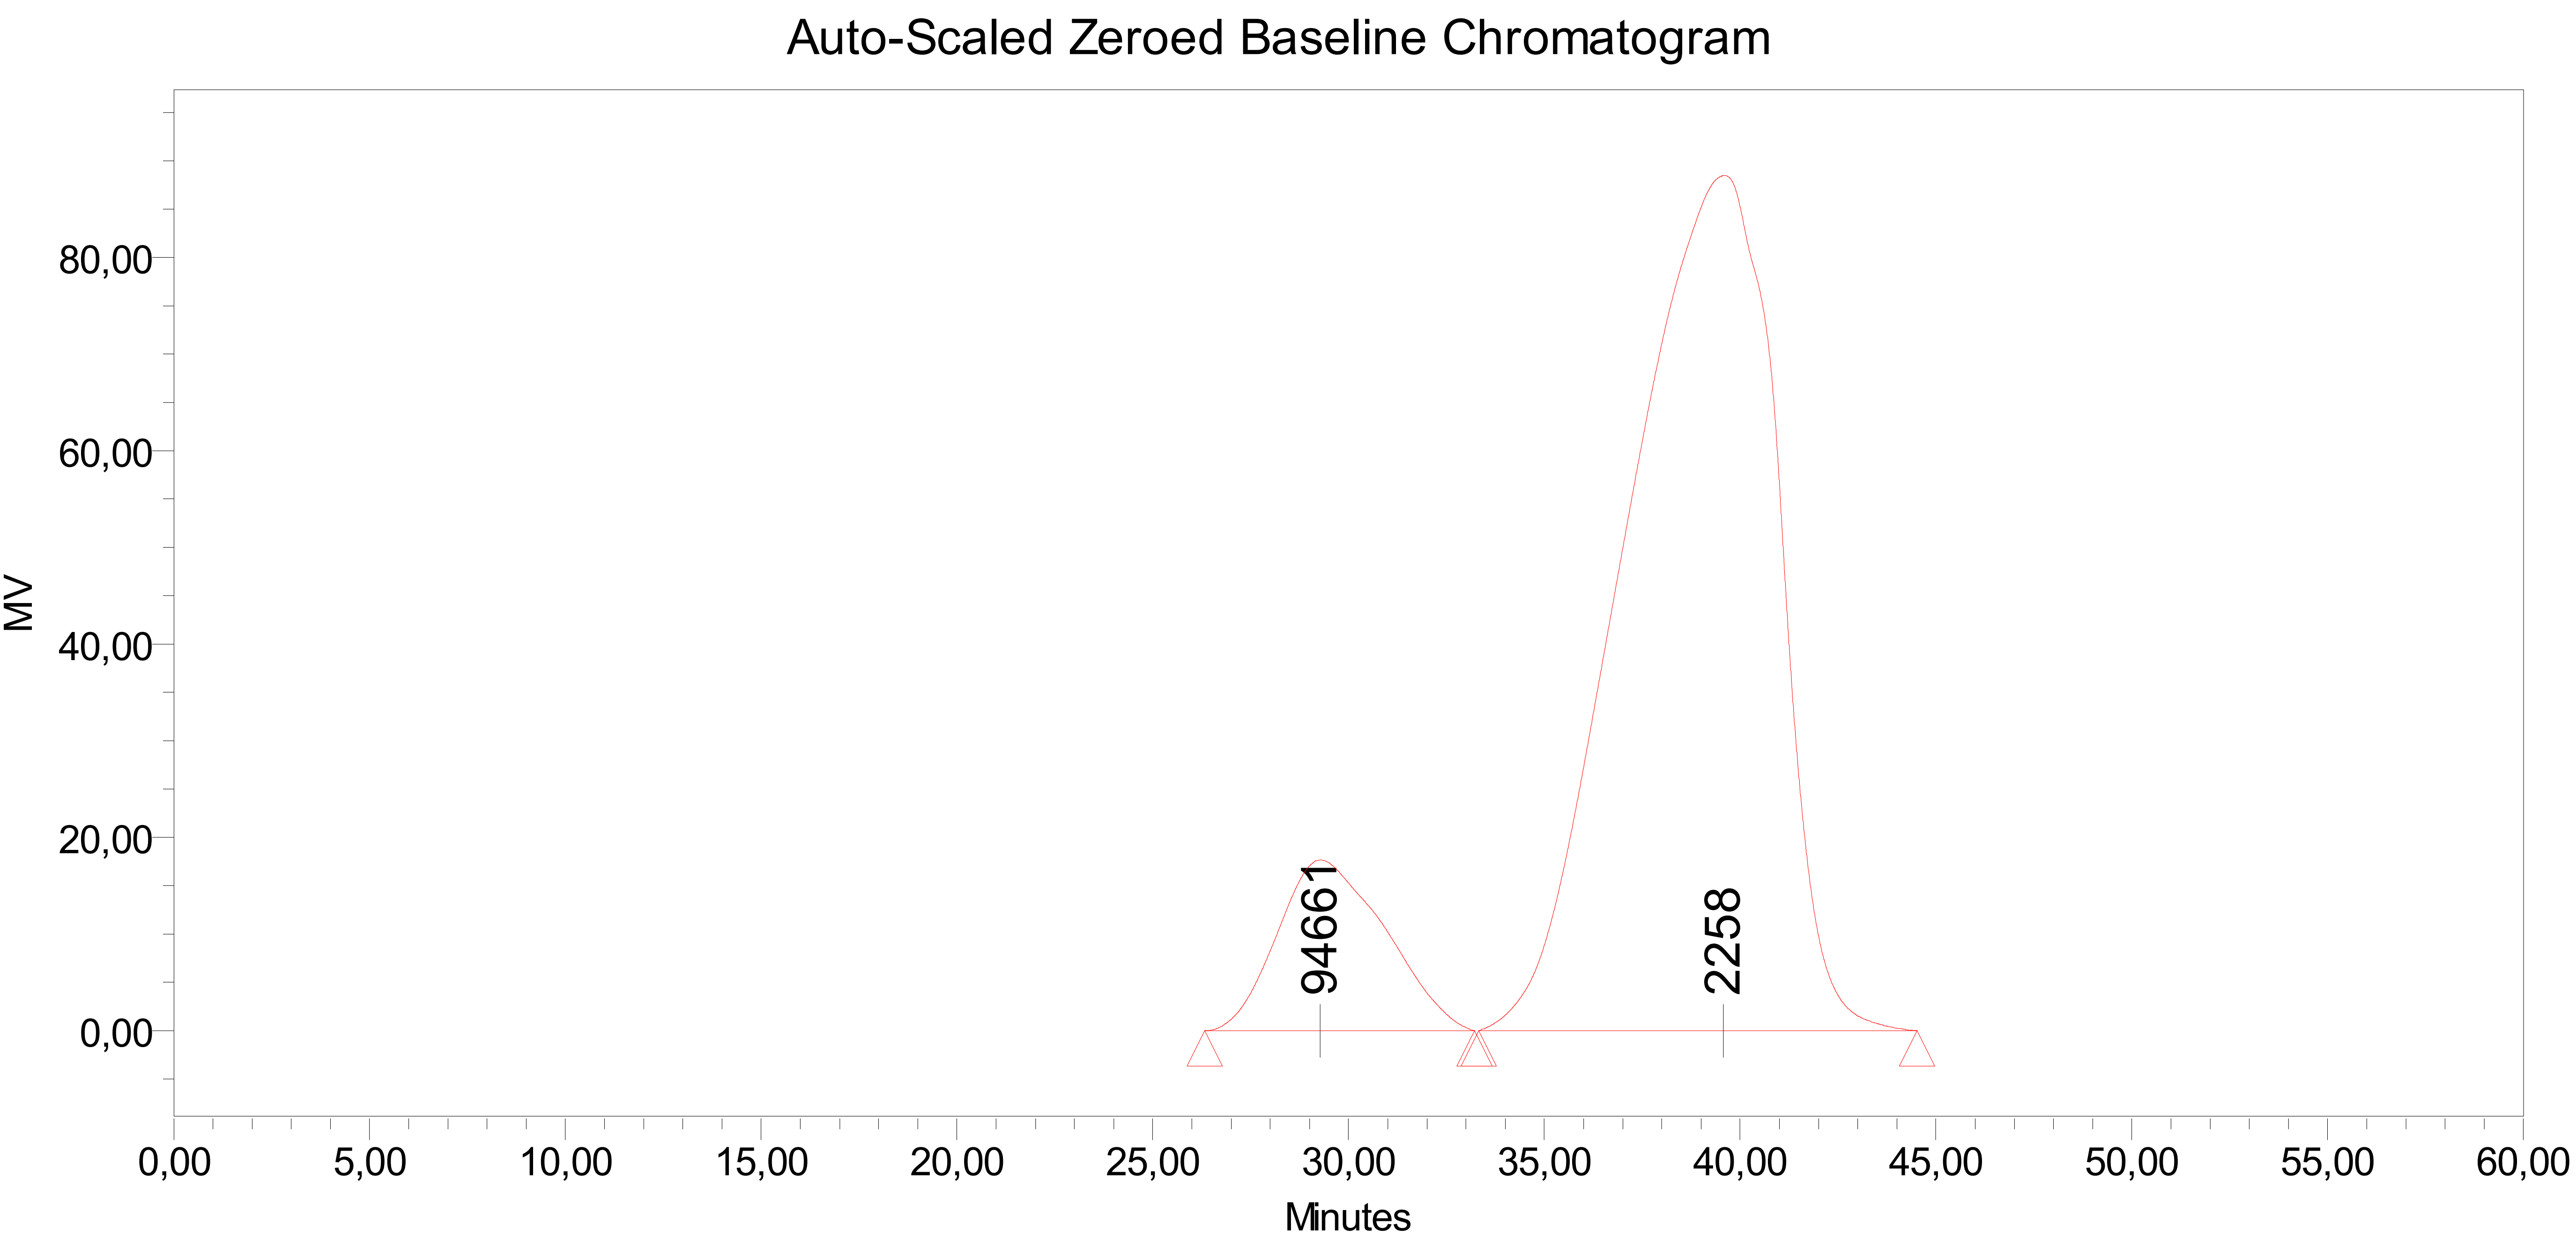

GPC Sample Results

	Retention Time	Mn	Mw	MP	Mz	Poly-dispersity	%Area
1	29,273	63466	96305	94661	144288	1,517	12,42
2	39,573	2503	3235	2258	4292	1,292	87,58

GPC Calibration Plot

